

YDK010/pPK4-HCP ELISA

Enzyme immunoassay for the quantitative determination of Host Cell Protein (HCP) originating from Corynex[®] System in cell culture supernatant.

REF **30116226**

 **12 x 8**

For illustrative purposes only.

To perform the assay the instructions for use provided with the kit have to be used.

Distributed by:

I B L I N T E R N A T I O N A L G M B H
Flughafenstrasse 52a Phone: +49 (0)40-53 28 91-0 IBL@IBL-International.com
D-22335 Hamburg, Germany Fax: +49 (0)40-53 28 91-11 www.IBL-International.com

YDK010/pPK4-HCP Assay Kit - IBL

96 Well

Please read carefully this instruction prior you use this assay kit.

INSTRUCTIONS FOR USE

This product is for research use only and is not intended for diagnostic use.

KIT COMPONENT

1	Precoated plate: (Anti-YDK010/pPK4-HCP Rabbit IgG)	96Well x 1
2	Labeled antibody conc.: (30X) HRP conjugated Anti- YDK010/pPK4-HCP Rabbit IgG Fab'	0.4mL x 1
3	Standard: (YDK010/pPK4-HCP)	0.5mL x 2
4	EIA buffer	30mL x 1
5	Solution for labeled antibody	12mL x 1
6	Chromogen: TMB solution	15mL x 1
7	Stop solution	12mL x 1
8	Wash buffer conc.	50mL x 1

MEASURING SAMPLES

This kit can measure HCP (Host Cell Protein) originated from cell culture medium using Corynex® System*. HCP originated from cell culture medium in cell culture supernatant, intermediate purified product and finished purified product can be detected by this kit.

Corynex® System: This is a protein/peptide secretion expression system (Corynebacterium Expression System) using gram-positive bacteria *Corynebacterium glutamicum*.

PRINCIPLE

This kit is a solid phase sandwich ELISA (Enzyme-linked Immunosorbent Assay). As a primary antibody is coated on a plate, samples and standard are added into the wells for 1st reaction. After the reaction, HRP-conjugated secondary antibody is added into the wells for 2nd reaction. After washing away unbound the secondary antibody, Tetra Methyl Benzidine (TMB) is added to the wells and color develops.

OPERATING PRECATION

- Test samples should be measured soon after collection. For storage of samples, store them frozen and do not repeat freeze/thaw cycles. Thaw the test samples at a low temperature and mix them completely before measurement.
- Test samples should be diluted with "4, EIA buffer" contained in this kit.
- Duplicate measurement of test samples and standards is recommended.
- Standard curve should run for each assay.
- Use test samples in neutral pH range. The contaminations of organic solvent may affect the measurement.
- All reagents should be brought to room temperature (R.T.) and mixed completely and gently before use. After mixing them, make sure of no change in quality of the reagents.
- Use only "8, Wash buffer conc." contained in this kit for washing the precoated plate. Insufficient washing may lead to the failure in measurement.
- Fill the wash buffer each well, invert the plate and make sure the liquid is completely removed by shaking it off if you use a washing bottle. Repeat this washing process several times as instructed in order to avoid any insufficient washing process.
- After remove the wash buffer, tapping the plate against a clean paper towel for completely removing the liquid from the wells and make sure the paper towel is not contact with inside of the wells in this process.
- "6, Chromogen - TMB solution" should be stored in the dark due to its sensitivity against light. It should be also avoided contact with metals. Required quantity should be prepared into a collecting container for each use.
- After adding TMB solution into the wells, the liquid in the wells gradually changes the color in blue. In this process the plate should be in dark. Remained TMB solution in the collecting container should not be returned into the original bottle of TMB solution to avoid contamination.
- Measurement of O.D. should be done within 30 minutes after addition of "7, Stop solution".

OPERATION MANUAL AND DOSAGES

1. Materials needed but not supplied.

Plate reader	Micropipette and tip
Test tubes for dilution	Measuring cylinder and beaker
Deionized water	Plate washer
Paper towel	Collecting container
Refrigerator	(i.e. clean disposable test tube)
	Incubator (37°C±1°C)

2. Preparation

(1) Preparation of wash buffer
Dilute "8, Wash buffer conc." 40 fold with deionized water. The diluted one is used for the assay as a wash buffer. Adjust the required quantities if needed.

(2) Preparation of labeled antibody
Dilute "2, Labeled antibody conc." 30 fold with "5, Solution for labeled antibody" using a prepared collecting container.

(3) Preparation of standard
Add 0.5 mL of deionized water into the vial of "3, Standard" and completely dissolve it. Concentration of the standard is 4000 pg/mL. The standards enclosed in this kit can be frozen and stored after reconstitution. However the freeze-thaw shall not be repeated.

Prepare 7 test tubes for dilution of the standard and adding 230 µL of the EIA buffer into each tube.

Put 230 µL of 4000 pg/mL standard into the tube 2000 pg/mL (Tube-1) and gently mix it. Afterword, put 230 µL of the mixed liquid of tube-1 into the tube 1000 pg/mL (Tube-2) and gently mix it. Dilute two fold standard solution in series to set up 7 points of diluted standard between 31.25 pg/mL ~ 2000 pg/mL.

Tube-1	2000	pg/mL
Tube-2	1000	pg/mL
Tube-3	500	pg/mL
Tube-4	250	pg/mL
Tube-5	125	pg/mL
Tube-6	62.50	pg/mL
Tube-7	31.25	pg/mL

(4) Preparation of test samples
Dilute test samples with "4, EIA buffer" contained in this kit as follows.
Recommended dilution ratio: more than 4 fold.

3 MEASUREMENT PROCEDURE

(1) Add test sample blank
Determine wells for test sample blank. Put 100µL each of "4, EIA buffer" into the wells.

(2) Add prepared test samples and standard
Put 100 µL prepared test samples and 100 µL prepared standard into appropriate wells.

(3) Incubation with plate lid (1st reaction).

(4) Washing
Wash the plate with the prepared wash buffer and remove all liquid.

(5) Add prepared labeled antibody
Put 100 µL prepared labeled antibody into the wells.

(6) Incubation with plate lid (2nd reaction).

(7) Washing
Wash the plate with the prepared wash buffer and remove all liquid completely.

(8) Add "6, Chromogen - TMB solution"

Put 100 µL the TMB solution into the wells.

(9) Incubation in dark

(10) Add "7, Stop solution"

Put 100 µL the Stop solution into the wells.

(11) Determination of optical density (O.D.)

Remove any dirt or drop of water on the bottom of the plate and confirm there is no bubble on the surface of the liquid. Then, measure the both O.D. of standard and the test samples against a test sample blank.

Measurement wavelength: 450 nm. In case of 2 wavelengths:

Main wavelength is 450nm. Sub-wavelength is between 600 and 650 nm.


Table for measurement procedure

	Test samples	Standard	Test sample blank
Reagents	Test samples 100 µL	Diluted Standard 100 µL	EIA buffer 100 µL
1st reaction	Incubation for 60 minutes 37°C with plate lid.		
Washing	4 times (wash buffer more than 350 µL)		
Labeled antibody	100 µL	100 µL	100 µL
2nd reaction	Incubation for 30 minutes 37°C with plate lid.		
Washing	5 times (wash buffer more than 350 µL)		
TMB solution	100 µL	100 µL	100 µL
Chromogenic reaction	Incubation for 30 minutes at R.T. (shielded).		
Stop solution	100 µL	100 µL	100 µL
Measuring O.D.	450 nm / 600~650 nm		

CALCULATION OF TEST RESULT

- Plot the concentration of the standard on the x-axis and its O.D. on the y-axis. Draw a standard curve by applying appropriate regression curve on each plot (i.e. quadratic regression of double logarithm conversion).
- Read the concentration by applying the absorbance of the test samples on a standard curve.
- Calculate the concentration of the test samples by multiplying dilution ratio of test samples on the value.

Example of standard curve and measured value

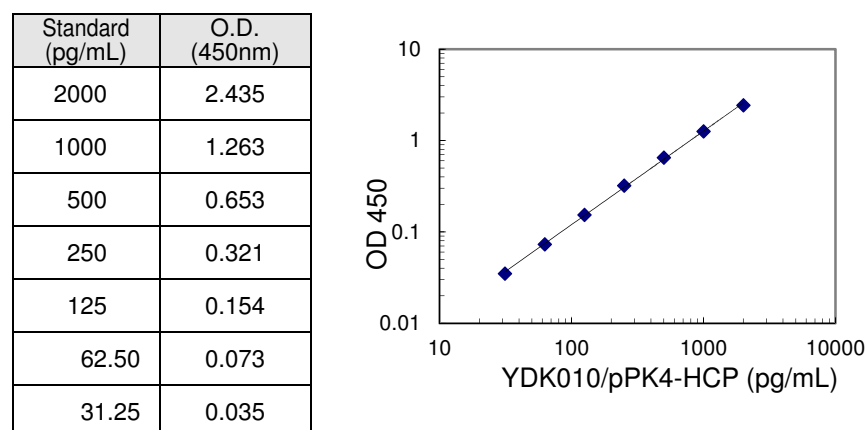

PERFORMANCE AND CHARACTERISTICS



1 Sensitivity

3.57 pg/mL

2 Measurement range

31.25 ~ 2000 pg/mL

3 Dilution linearity

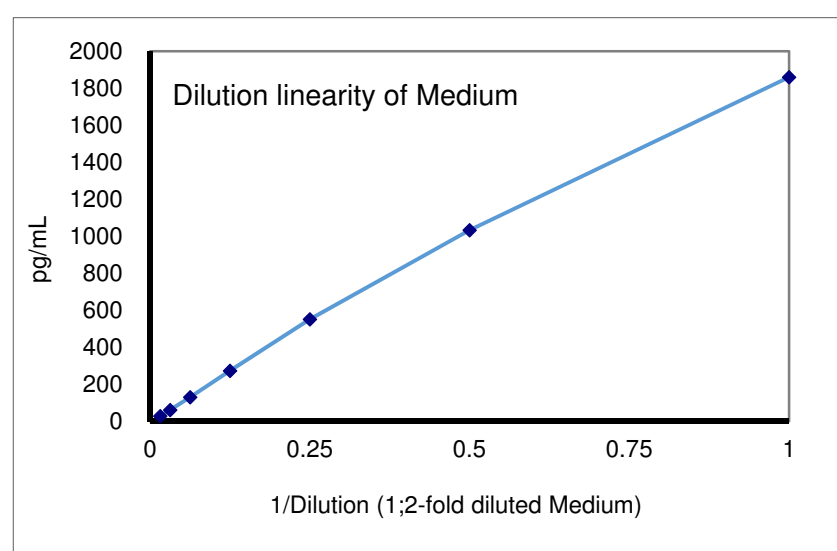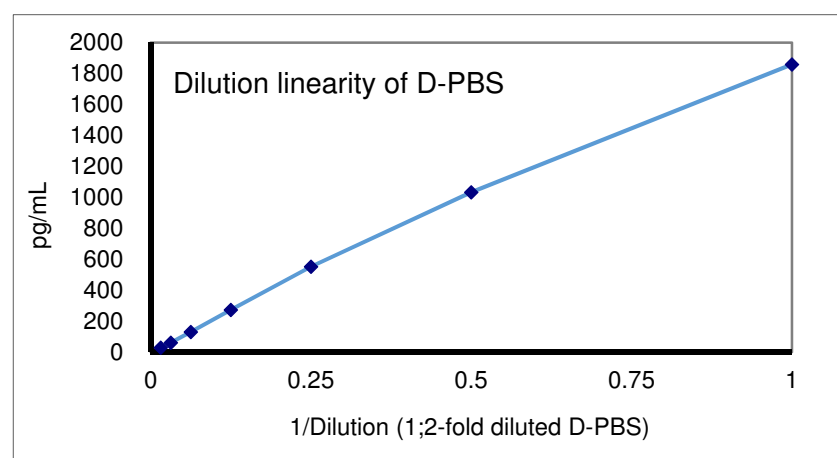

4 Added recovery assay

Specimen	Added Volume (pg/mL)	Theoretical Value (pg/mL)	Measurement Value (pg/mL)	%
D-PBS(x1)	1000	1000	961.03	96.1
	500	500	496.61	99.3
	250	250	254.10	101.6
	125	125	122.44	98.0
Medium (x50)	1000	1000	964.26	96.4
	500	500	491.84	98.4
	250	250	249.77	99.9
	125	125	122.02	97.6

5 Intra-assay

Measurement value (pg/mL)	SD (pg/mL)	CV (%)	n
987.29	28.63	2.9	8
209.87	11.81	5.6	8
80.47	7.22	9.0	8

6 Inter-assay

Measurement value (pg/mL)	SD (pg/mL)	CV (%)	n
998.32	47.76	4.8	8
204.16	10.08	4.9	8
82.44	5.88	7.1	8

7 Specificity

Substance	Cross reactivity (%)
YDK010/pPK4-HCP	100
Medium	N.D.
PBS	N.D.

PRECAUTION FOR INTENDED USE AND/OR HANDLING

1 Precaution for handling (Hazard prevention)

- Treat the components carefully and wash hands after handling it.
- "7, Stop solution" is a strong acid substance (1N Sulfuric acid). Therefore, it should be careful for the treatment and do not contact your skin and clothes with it. It also needs to pay attention to the disposal of it.

2 Precaution for intended use

- "3, Standard" is lyophilized products. It should be careful to open this vial.
- All reagents should be stored at 2 - 8°C.
- Precipitation can be seen in "4, EIA buffer", "5, Solution for labeled antibody" and "8, Wash buffer conc.", however, it does not affect its performance.
- Do not mix or replace the reagents with the reagents from a different lot or kit.
- Do not use expired reagents.

3 Precaution for disposal

- Dispose used materials after rinsing them with large quantity of water.

STORAGE AND THE TERM OF VALIDITY

Storage Condition: 2 - 8°C

The expiry date is specified on the outer box.

PACKAGE UNIT AND PRODUCT NUMBER

Package unit: 96 Well

Product number: 27800














REFERENCES

- Kikuchi, Y., M. Date, K. Yokoyama, Y. Umezawa, and H. Matsui. (2003) Secretion of active-form Streptovorticillium mobaraense transglutaminase by Corynebacterium glutamicum: processing of the pro-domain by a co-secreted subtilisin-like protease from Streptomyces albogriseolus. Appl. Environ. Microbiol. 69:358-366.
- Kikuchi, Y., Itaya, H., Date, M., Matsui, K., and Wu, L.-F. (2009) TatABC overexpression improves Tat-dependent protein secretion in Corynebacterium glutamicum. Appl. Environ. Microbiol. 75:603-607.

CONTACT DETAILS

Immuno-Biological Laboratories Co., Ltd.
 1091-1 Naka, Fujioka-Shi, Gunma 375-0005
 TEL : 0274-22-2889
 FAX : 0274-23-6055

Symbols / Symbole / Symbôles / Símbolos / Símbolos / Σύμβολα

	Cat.-No.: / Kat.-Nr.: / No.- Cat.: / Cat.-No.: / N.º Cat.: / N.-Cat.: / Αριθμός-Κατ.:
	Lot-No.: / Chargen-Bez.: / No. Lot: / Lot-No.: / Lote N.º: / Lotto n.: / Αριθμός -Παραγωγή:
	Use by: / Verwendbar bis: / Utiliser à: / Usado por: / Usar até: / Da utilizzare entro: / Χρησιμοποιείται από:
	No. of Tests: / Kitgröße: / Nb. de Tests: / No. de Determ.: / N.º de Testes: / Quantità dei tests: / Αριθμός εξετάσεων:
	Concentrate / Konzentrat / Concentré / Concentrar / Concentrado / Concentrato / Συμπύκνωμα
	Lyophilized / Lyophilisat / Lyophilisé / Liofilizado / Liofilizado / Liofilizzato / Λυοφιλιασμένο
	In Vitro Diagnostic Medical Device. / In-vitro-Diagnostikum. / Appareil Médical pour Diagnostics In Vitro. / Dispositivo Médico para Diagnóstico In Vitro. / Equipamento Médico de Diagnóstico In Vitro. / Dispositivo Medico Diagnostico In vitro. / Ιατρική συσκευή για In-Vitro Διάγνωση.
	Evaluation kit. / Nur für Leistungsbewertungszwecke. / Kit pour évaluation. / Juego de Reactivos para Evaluació. / Kit de avaliação. / Kit di evaluazione. / Κιτ Αξιολόγησης.
	Read instructions before use. / Arbeitsanleitung lesen. / Lire la fiche technique avant emploi. / Lea las instrucciones antes de usar. / Ler as instruções antes de usar. / Leggere le istruzioni prima dell'uso. / Διαβάστε τις οδηγίες πριν την χρήση.
	Keep away from heat or direct sun light. / Vor Hitze und direkter Sonneneinstrahlung schützen. / Garder à l'abri de la chaleur et de toute exposition lumineuse. / Manténgase alejado del calor o la luz solar directa. / Manter longe do calor ou luz solar directa. / Non esporre ai raggi solari. / Να φυλάσσεται μακριά από θερμότητα και άμεση επαφή με το φως του ηλίου.
	Store at: / Lagern bei: / Stocker à: / Almacene a: / Armazemar a: / Conservare a: / Αποθήκευση στους:
	Manufacturer: / Hersteller: / Fabricant: / Productor: / Fabricante: / Fabbicante: / Παραγωγός:
	Caution! / Vorsicht! / Attention! / ¡Precaución! / Cuidado! / Attenzione! / Προσοχή!
<p>Symbols of the kit components see MATERIALS SUPPLIED. Die Symbole der Komponenten sind im Kapitel KOMPONENTEN DES KITS beschrieben. Voir MATERIEL FOURNI pour les symbôles des composants du kit. Símbolos de los componentes del juego de reactivos, vea MATERIALES SUMINISTRADOS. Para símbolos dos componentes do kit ver MATERIAIS FORNECIDOS. Per i simboli dei componenti del kit si veda COMPONENTI DEL KIT. Για τα σύμβολα των συστατικών του κιτ συμβουλευτείτε το ΠΑΡΕΧΟΜΕΝΑ ΥΛΙΚΑ.</p>	

COMPLAINTS: Complaints may be submitted initially written or vocal. Subsequently they need to be filed including the test performance and results in writing in case of analytical reasons.

WARRANTY: The product is warranted to be free from material defects within the specific shelf life and to comply with product specifications delivered with the product. The product must be used according to the Intended use, all instructions given in the instructions for use and within the product specific shelf life. Any modification of the test procedure or exchange or mixing of components of different lots could negatively affect the results. These cases invalidate any claim for replacement.

LIMITATION OF LIABILITY: IN ALL CIRCUMSTANCES THE EXTENT OF MANUFACTURER'S LIABILITY IS LIMITED TO THE PURCHASE PRICE OF THE KIT(S) IN QUESTION. IN NO EVENT SHALL MANUFACTURER BE LIABLE FOR ANY INCIDENTAL OR CONSEQUENTIAL DAMAGES, INCLUDING DAMAGES FOR LOST PROFITS, LOST SALES, INJURY TO PERSON OR PROPERTY OR ANY OTHER INCIDENTAL OR CONSEQUENTIAL LOSS.

IBL International GmbH
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11
E-MAIL: IBL@IBL-International.com
WEB: <http://www.IBL-International.com>