

Instructions for Use



IBL International GmbH
Flughafenstraße 52 a
22335 Hamburg, Germany

Tel. +49 (0) 40 53 28 91-0
Fax +49 (0) 40 53 28 91-11

IBL@tecan.com
www.tecan.com/ibl

Vasoactive Intestinal Polypeptide (VIP) ELISA

For the quantitative measurement of Vasoactive Intestinal Polypeptide (VIP) in human EDTA plasma by an ELISA (Enzyme-Linked Immunosorbent Assay).

REF 30251374

 96

For illustrative purposes only.

To perform the assay the instructions for use provided with the kit have to be used

Distributed by: **IBL International GmbH**
Flughafenstrasse 52a
22335 Hamburg, Germany

Always there for you



Vasoactive Intestinal Polypeptide (VIP) ELISA

REF 30251374 (CAN-VIP-380)

RUO

Effective Date: August 22, 2024

Version: RUO-3.0

1. INTENDED PURPOSE & USE

For the quantitative measurement of Vasoactive Intestinal Polypeptide (VIP) in human EDTA plasma by an ELISA (Enzyme-Linked Immunosorbent Assay).

For Research Use Only. Not for use in diagnostic procedures.

2. LIMITATIONS RELATED TO INTENDED PURPOSE & USE

- This kit is intended for research use only and is not to be used for any diagnostic procedures.

3. PRINCIPLE OF THE TEST

The VIP ELISA is a two-step competitive immunoassay. In the first incubation step, competition occurs between VIP present in calibrators, controls, specimen samples and a biotin-labelled antigen (biotin conjugate) for a limited number of anti-VIP antibody binding sites on the microplate wells. Excess and unbound materials are removed by a washing step. In the second incubation step, streptavidin-HRP conjugate is added, which binds specifically to any bound biotin conjugate. After a washing step that removes unbound materials, the TMB substrate (enzyme substrate) is added which reacts with HRP to form a blue-coloured product that is inversely proportional to the amount of VIP present. Following an incubation, the enzymatic reaction is terminated by the addition of the stopping solution, converting the colour from blue to yellow. The absorbance is measured on a microplate reader at 450 nm. A set of calibrators is used to plot a calibrator curve from which the amount of VIP in specimen samples and controls can be directly read.

4. PROCEDURAL CAUTIONS AND WARNINGS

- This kit is for use by trained laboratory personnel (professional use only). For laboratory *in vitro* use only.
- Practice good laboratory practices when handling kit reagents and specimens. This includes:
 - Do not pipette by mouth.
 - Do not smoke, drink, or eat in areas where specimens or kit reagents are handled.
 - Wear protective clothing and disposable gloves.
 - Wash hands thoroughly after performing the test.
 - Avoid contact with eyes; use safety glasses; in case of contact with eyes, flush eyes with water immediately and contact a doctor.
- Users should have a thorough understanding of this protocol for the successful use of this kit. Reliable performance will only be attained by strict and careful adherence to the instructions provided.
- Do not use the kit beyond the expiry date stated on the label.
- If the kit reagents are visibly damaged, do not use the test kit.
- Do not use kit components from different kit lots within a test and do not use any component beyond the expiration date printed on the label.
- All kit reagents and specimens must be brought to room temperature and mixed gently but thoroughly before use. Avoid repeated freezing and thawing of specimens.
- When the use of water is specified for dilution or reconstitution, use deionized or distilled water.

- When adding deionized water for the reconstitution of lyophilized components, it is recommended to pre-wet the pipette tip to ensure an accurate transfer of water.
- Immediately after use, each individual component of the kit must be returned to the recommended storage temperature stated on the label. For reconstituted lyophilized reagents, follow storage requirements in section 8. *Reagents Provided*.
- A calibrator curve must be established for every run.
- It is recommended to all customers to prepare their own control materials or plasma pools which should be included in every run at a high and low level for assessing the reliability of results.
- The controls (included in kit) must be included in every run and their results must fall within the ranges stated in the quality control certificate; a failed control result might indicate improper procedural techniques or pipetting, incomplete washing, or improper reagent storage.
- When dispensing the substrate and stopping solutions, do not use pipettes in which these liquids will come into contact with any metal parts.
- The TMB Substrate is sensitive to light and should remain colourless if properly stored. Instability or contamination may be indicated by the development of a blue colour, in which case it should not be used.
- Do not use grossly hemolyzed, grossly lipemic, icteric or improperly stored plasma.
- Samples or controls containing azide or thimerosal are not compatible with this kit, they may lead to false results.
- Samples values above the measuring range of the kit may be reported as >800 pg/mL. If further dilution and retesting is required, only the Assay Buffer may be used to dilute EDTA plasma samples. The use of any other reagent may lead to false results.
- Avoid microbial contamination of reagents.
- To prevent the contamination of reagents, use a new disposable pipette tip for dispensing each reagent, sample, calibrator, and control.
- To prevent the contamination of reagents, do not pour reagents back into the original containers.
- Kit reagents must be regarded as hazardous waste and disposed of according to local and/or national regulations.
- Consumables used with the kit that are potentially biohazardous (e.g., pipette tips, bottles or containers containing human materials) must be handled according to biosafety practices to minimize the risk of infection and disposed of according to local and/or national regulations relating to biohazardous waste.
- This kit contains 1 M sulfuric acid in the stopping solution component. Do not combine acid with waste material containing sodium azide or sodium hypochlorite.
- The use of safety glasses, and disposable plastic, is strongly recommended when manipulating biohazardous or bio-contaminated solutions.
- Proper calibration of the equipment used with the test, such as the pipettes and absorbance microplate reader, is required.
- If a microplate shaker is required for the assay procedure, the type and speed of shaker required is stated in the REAGENTS AND EQUIPMENT NEEDED BUT NOT PROVIDED section. Both the type and speed of shaker used can influence the optical densities and test results. If a different type of shaker and/or speed is used, the user is responsible for validating the performance of the kit.
- Do not reuse the microplate wells, they are for SINGLE USE only.
- To avoid condensation within the microplate wells in humid environments, do not open the pouch containing the microplate until it has reached room temperature.
- When reading the microplate, the presence of bubbles in the wells will affect the optical densities (ODs). Carefully remove any bubbles before performing the reading step.

5. SAFETY CAUTIONS AND WARNINGS

5.1 BIOHAZARDS

The reagents should be considered a potential biohazard and handled with the same precautions applied to blood specimens. All human specimens should be considered a potential biohazard and handled as if capable of transmitting infections and in accordance with good laboratory practices.

The calibrator stock, controls and assay buffer provided with the kit contain processed human serum/plasma that has been tested by approved methods and found to be negative for the presence of HBsAg and antibodies to HCV, HIV 1/2 and HIV NAT. However, no test method can offer complete assurance that any viable pathogens are absent. Therefore, these components should be considered a potential biohazard and handled with the same precautions as applied to any blood specimen, following good laboratory practices.

5.2 CHEMICAL HAZARDS

Avoid direct contact with any of the kit reagents. Specifically avoid contact with the TMB Substrate (contains tetramethylbenzidine) and Stopping Solution (contains sulfuric acid). If contacted with any of these reagents, wash with plenty of water and refer to SDS for additional information.

6. SPECIMEN COLLECTION, STORAGE AND PRE-TREATMENT

6.1 Specimen Collection & Storage



Follow the specimen collection procedure steps in the order provided below to avoid any delays that could potentially affect the stability of specimen samples. K2 and K3 EDTA collection tubes are suitable for plasma sample collection.

Approximately 0.2 mL of K2 or K3 EDTA plasma is required per duplicate determination.

- Prior to sample collection, place a K2 or K3 EDTA plasma collection tube into a container of ice for at least 10 minutes.
- Collect 4–5 mL of venous blood into an appropriately labelled pre-cooled EDTA plasma collection tube.
- Mix the tube by inverting several times.
- Place the collection tube into a container of ice to keep cool prior to centrifugation.
- Centrifuge the tube at 2000x g for 10 minutes and carefully transfer the plasma into a new storage tube or container.
- If the sample will not be tested immediately, the plasma should be aliquoted and stored frozen at ≤ -20°C for up to 3 months. Repeated freezing and thawing should be avoided.

Consider all human specimens as possible biohazardous materials and take appropriate precautions when handling.

6.2 Specimen Pre-Treatment

Specimen pre-treatment is not required.

7. REAGENTS AND EQUIPMENT NEEDED BUT NOT PROVIDED

- Calibrated single-channel pipette to dispense 40 – 100 µL and 500 – 1000 µL.
- Calibrated multi-channel pipettes to dispense 25 µL, 50 µL and 150 µL.
- Calibrated multi-channel pipettes to dispense 350 µL (if washing manually).
- Automatic microplate washer (recommended).
- Microplate shaker: Orbital shaker (3 mm shaking diameter) set to 600 rpm.
- Disposable pipette tips.
- Distilled or deionized water.
- Calibrated absorbance microplate reader with a 450 nm filter and an upper OD limit of 3.0 or greater.
- Polypropylene or HDPE tubes for calibrator preparation (e.g. polypropylene microcentrifuge tubes).
- Centrifuge capable of 2000x g.
- Container with ice.
- Vortex mixer.

8. REAGENTS PROVIDED


MPL	Microplate
Contents:	One anti-VIP polyclonal antibody-coated 96-well (12x8) microplate in a resealable pouch with desiccant.
Format:	Ready to Use
Storage:	2–8°C
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening: Stable for six weeks.

BIOT	CONJ	CONC	LYO	Biotin Conjugate Concentrate Lyophilized		
Contents:	One bottle containing lyophilized VIP-Biotin conjugate in a protein-based buffer with a non-mercury preservative.					
Format:	Lyophilized and Concentrated; Requires Preparation					
Storage:	2–8°C					
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening and Reconstitution: Stable for 1 month at 2–8°C. For long-term storage, store at ≤ -20°C for up to 3 months with no more than 3 freeze/thaw cycles. Following Preparation: The Biotin Conjugate Working Solution is stable for 2 hours at room temperature following preparation. Discard the working solution after use; do not store for future use.					
Reconstitution:	Reconstitute the lyophilized Biotin Conjugate by adding 0.5 mL of distilled or deionized water to the bottle. Replace the stopper and let stand at room temperature for 10 minutes. Mix gently without foaming before use.					
Preparation of Biotin Conjugate Working Solution:	<table border="1" style="width: 100%;"> <tr> <td>X101</td> <td>Dilute 1:101 Before Use</td> </tr> </table> <p>Dilute the reconstituted Biotin Conjugate 1:101 in Assay Buffer (e.g., 40 µL of reconstituted Biotin Conjugate in 4 mL of Assay Buffer) and vortex to mix. If the whole plate is to be used dilute 80 µL of reconstituted Biotin Conjugate in 8 mL of Assay Buffer and vortex to mix. Return unused reconstituted Biotin Conjugate back to 2–8°C or ≤ -20°C storage conditions (see stability section above).</p>				X101	Dilute 1:101 Before Use
X101	Dilute 1:101 Before Use					

3. **STA HRP CONJ** Streptavidin HRP Conjugate

Contents:	One bottle containing Streptavidin-Horse Radish Peroxidase (HRP) conjugate in a stabilized buffer with a non-mercury preservative.
Format:	Ready to Use
Volume:	20 mL/bottle
Storage:	2-8°C
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening: Stable for six weeks.

4. **CAL STK LYO** Calibrator Stock Lyophilized

Contents:	One bottle of calibrator stock containing VIP in a human plasma-based buffer with a non-mercury preservative. Used for the preparation of VIP calibrators.
Format:	Lyophilized and Concentrated; Requires Preparation
Storage:	2-8°C (unopened)
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening and Reconstitution: Store remaining reconstituted Calibrator Stock at ≤ -20°C for up to 1 month with no more than 2 freeze/thaw cycles.
Reconstitution:	Reconstitute the lyophilized Calibrator Stock by adding 0.5 mL of distilled or deionized water to the bottle. Replace the stopper and let stand at room temperature for 2 minutes. Mix gently without foaming before use.
	 Only reconstitute the Calibrator Stock immediately prior to the preparation of VIP Calibrators.
Preparation of Calibrators:	See section 9. Preparation of VIP Calibrators.

5. **CONTROL 1-2 LYO** Control 1 – 2 Lyophilized

Contents:	Two bottles of lyophilized control containing different VIP concentrations. Human plasma-based buffer with a non-mercury preservative. Prepared by spiking buffer with defined quantities of VIP. Refer to the QC certificate for the target values and acceptable ranges.
Format:	Lyophilized; Requires Preparation
Storage:	2-8°C (unopened)
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening and Reconstitution: Stable for 2 hours at room temperature. For long-term storage, store at ≤ -20°C for up to 1 month with no more than 2 freeze/thaw cycles.
Reconstitution:	Reconstitute each bottle of control (Control 1 & Control 2) by adding 0.5 mL of distilled or deionized water to the bottle. Replace the stopper and let stand at room temperature for 2 minutes. Mix gently without foaming.

6. **INC BUFF** Incubation Buffer

Contents:	One bottle containing a protein-based buffer with a non-mercury preservative.
Format:	Ready to Use
Volume:	6 mL/bottle
Storage:	2-8°C
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening: Stable for six weeks.


7. **ASY BUFF** Assay Buffer

Contents:	One bottle containing a human plasma-based buffer with a non-mercury preservative. Used for the preparation of the VIP calibrators and the Biotin Conjugate Working Solution.
Format:	Ready to Use
Volume:	20 mL/bottle
Storage:	2-8°C
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening: Stable for six weeks.

8. **TMB SUB** TMB Substrate

Contents:	One bottle containing tetramethylbenzidine and hydrogen peroxide in a non-DMF or DMSO containing buffer.
Format:	Ready to Use
Volume:	18 mL/bottle
Storage:	2-8°C
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening: Stable for six weeks.

9. **STOP** Stopping Solution

Contents:	One bottle containing 1M sulfuric acid.
Format:	Ready to Use
Volume:	8 mL/bottle
Storage:	2-8°C
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening: Stable for six weeks.
Safety:	 Refer to product SDS. Warning


10. **WASH BUFF CONC** Wash Buffer Concentrate

Contents:	One bottle containing buffer with a non-ionic detergent and a non-mercury preservative.
Format:	Concentrated; Requires Preparation
Volume:	50 mL/bottle
Storage:	2-8°C
Stability:	Unopened: Stable until the expiry date printed on the label. After Opening: Stable for six weeks. Following Preparation: The wash buffer working solution is stable for 2 weeks following preparation, assuming Good Laboratory Practices are adhered to. To prevent microbial growth, prepare the wash buffer working solution in a clean container and store under refrigerated conditions (2-8°C) when not in use.
Preparation of Wash Buffer Working Solution:	X10 Dilute 1:10 Before Use Dilute 1:10 in distilled or deionized water before use. If the whole microplate is to be used dilute 50 mL of the wash buffer concentrate in 450 mL of distilled or deionized water.


9. PREPARATION OF VIP CALIBRATORS

Materials Required:


- Calibrator Stock.
- Assay Buffer.
- Calibrated single-channel pipettes.
- 7 x polypropylene or HDPE tubes. (e.g. polypropylene microcentrifuge tubes).

 **Do not use glass test tubes; VIP may bind to glass which can alter the results.**

Procedure:

 **An accurate preparation of the calibrators is essential to the performance of the test. Please follow good pipetting practices specific to the brand of pipettes being used.**


- Label 7 x polypropylene or HDPE tubes as A, B, C, D, E, F & G, representing calibrators A-G.
- Pipette 960 µL of Assay Buffer to tube G.
- Pipette 500 µL of Assay Buffer to each tube A - F.
- Reconstitute the Calibrator Stock as stated in section 8. *Reagents Provided, 4. Calibrator Stock Lyophilized.*
- Pipette 40 µL of reconstituted Calibrator Stock to tube G. Vortex the tube to mix thoroughly.
- Immediately store the reconstituted Calibrator Stock at ≤ -20°C for future use.
- Pipette 500 µL from tube G into tube F. Vortex tube F to mix thoroughly.
- Pipette 500 µL from tube F into tube E. Vortex tube E to mix thoroughly.
- Pipette 500 µL from tube E into tube D. Vortex tube D to mix thoroughly.
- Pipette 500 µL from tube D into tube C. Vortex tube C to mix thoroughly.
- Pipette 500 µL from tube C into tube B. Vortex tube B to mix thoroughly.

 **Use the prepared VIP calibrators within 2 hours after preparation. Discard any leftover calibrators; do not store for future use.**





Preparation Summary Table

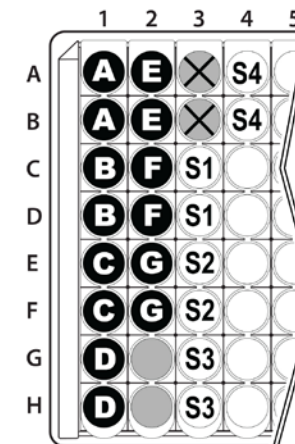Calibrator	VIP (pg/mL)	Assay Buffer	Calibrator
Calibrator Stock Reconstituted	-	-	-
G	800	960 µL	40 µL of Calibrator Stock
F	400	500 µL	500 µL of G
E	200	500 µL	500 µL of F
D	100	500 µL	500 µL of E
C	50	500 µL	500 µL of D
B	25	500 µL	500 µL of C
A	0	500 µL	-


10. RECOMMENDED ASSAY LAYOUT



Legend

-  Calibrators
-  Control 1
-  Control 2
-  Samples

11. ASSAY PROCEDURE

 Follow the assay procedure steps in the order provided below to avoid any delays that could potentially affect the stability of components and specimen samples.

All kit components, controls and specimen samples must reach room temperature prior to use. Calibrators, controls, and specimen samples should be assayed in duplicate. Once the procedure has been started, all steps should be completed without interruption.

- After all kit components have reached room temperature, **mix** gently by inversion.
- Plan** the microplate wells to be used for calibrators, controls, and samples. See section 10. *Recommended Assay Layout*. Remove the strips from the microplate frame that will not be used and place them in the bag with desiccant. Reseal the bag with the unused strips and return it to the refrigerator.
- Prepare** the Biotin Conjugate Working Solution and Wash Buffer Working Solution (See section 8. *Reagents Provided*, 2. *Biotin Conjugate Concentrate Lyophilized* and 10. *Wash Buffer Concentrate*).
- Prepare** the VIP Calibrators and Controls (See section 9. *Preparation of VIP Calibrators* and section 8. *Reagents Provided*, 4. *Calibrator Stock Lyophilized*, 5. *Control 1-2 Lyophilized*).
- Pipette 25 µL** of the Incubation Buffer into each well (the use of a multi-channel pipette is recommended).
- Pipette 75 µL** of each calibrator, control, and specimen sample into assigned wells.
- Incubate** the microplate on a microplate shaker** for **30 minutes** at room temperature.
- Pipette 50 µL** of the Biotin Conjugate Working Solution into each well (the use of a multi-channel pipette is recommended). **Avoid touching the liquid in the wells with the pipette tips.**
- Incubate** the microplate on a microplate shaker** for **60 minutes** at room temperature. Return leftover specimens to frozen storage at ≤ -20°C.
- Wash** the microplate wells with an automatic microplate washer (preferred) or manually as stated below.
Automatic: Using an automatic microplate washer, perform a **3-cycle** wash using **350 µL/well** of Wash Buffer Working Solution (3 x 350 µL). One cycle consists of aspirating all wells then filling each well with 350 µL of Wash Buffer Working Solution. After the final wash cycle, aspirate all wells and then tap the microplate firmly against absorbent paper to remove any residual liquid.
Manually: Perform a **3-cycle** wash using **350 µL/well** of Wash Buffer Working Solution (3 x 350 µL). One cycle consists of aspirating all wells by briskly emptying the contents of the wells over a waste container, then pipetting 350 µL of Wash Buffer Working Solution into each well using a multi-channel pipette. After the final wash cycle, aspirate all wells by briskly emptying the contents over a waste container and then tap the microplate firmly against absorbent paper to remove any residual liquid.
- Pipette 150 µL** of the Streptavidin HRP Conjugate into each well (the use of a multi-channel pipette is recommended).
- Incubate** the microplate on a microplate shaker** for **30 minutes** at room temperature.
- Wash** the microplate wells again as stated in step 10.
- Pipette 150 µL** of TMB Substrate into each well (the use of a multi-channel pipette is recommended).
- Incubate** the microplate on a microplate shaker** for **30 minutes** at room temperature.
- Pipette 50 µL** of Stopping Solution into each well (the use of a multi-channel pipette is recommended) in the same order and speed as was used for addition of the TMB Substrate. Gently tap the microplate frame to mix the contents of the wells.
- Measure** the optical density (absorbance) in the microplate wells using an absorbance microplate reader set to 450 nm, within 20 minutes after addition of the Stopping Solution.

** See section 7. *Reagents And Equipment Needed But Not Provided* for microplate shaker options.

12. CALCULATIONS

- Calculate the mean optical density for each calibrator, control and specimen sample duplicate.
- Use a 4-parameter or 5-parameter curve fit with immunoassay software to generate a calibrator curve.
- The immunoassay software will calculate the concentrations of the controls and specimen samples using the mean optical density values and the calibrator curve.
- If a sample reads more than 800 pg/mL and needs to be diluted and retested, then dilute with Assay Buffer not more than 1:5. The result obtained must be multiplied by the dilution factor.

13. QUALITY CONTROL

When assessing the validity of the test results, the following criteria should be evaluated:

- The calibrator A mean optical density meets the acceptable range as stated in the QC Certificate.
- The calibrator with the highest concentration meets the % binding acceptable range as stated in the QC Certificate.
% Binding = (OD of calibrator/OD of calibrator A) x 100.
- The values obtained for the kit controls are within the acceptable ranges as stated in the QC certificate.
- The results of any external controls that were used meet the acceptable ranges.

14. TYPICAL DATA


14.1 TYPICAL TABULATED DATA

Sample data only. **Do not** use to calculate results.












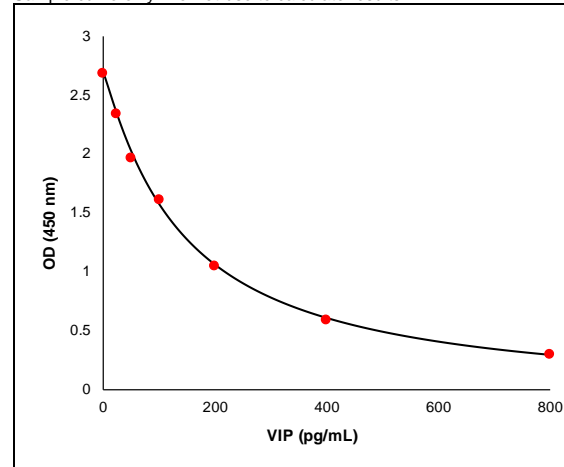








Calibrator	Mean OD (450 nm)	% Binding	Value (pg/mL)
A	2.684	100	0
B	2.346	87	25
C	1.969	73	50
D	1.613	60	100
E	1.055	39	200
F	0.595	22	400
G	0.305	11	800
Unknown	1.894	-	62.0

14.2 TYPICAL CALIBRATOR CURVE

Sample curve only. **Do not** use to calculate results.



15. SYMBOLS GLOSSARY

Symbol	Definition	Symbol	Definition
	Catalogue number		Manufacturer
	Batch code		Date of manufacture
	In vitro diagnostic medical device		Biological risks
	Unique Device Identifier		Consult instructions for use
	Dilute 1:# Before Use		Prescription only: Device restricted to use by or on the order of a physician
	Quantity		Keep away from sunlight
	Use-by date		Authorized representative in the European Community/ European Union
	Do not re-use		Temperature limit
	Caution		Contains sufficient for <n> tests
	Lyophilized		For Research Use Only. Not for use in diagnostic procedures.

The definitions of symbols used for kit component names are described in the *Reagents Provided* section.

16. CHANGE HISTORY

Previous Version:	RUO-2.0	New Version:	RUO-3.0
	6. SPECIMEN COLLECTION, STORAGE AND PRE-TREATMENT 6.1 Specimen Collection & Storage Warning Text Addition K2 and K3 EDTA collection tubes are suitable for plasma sample collection. Addition Approximately 0.2 mL of K2 or K3 EDTA plasma is required per duplicate determination. Changes: Addition 1. Prior to sample collection, place a K2 or K3 EDTA plasma collection tube into a container of ice for at least 10 minutes. Deletion 4. Samples should not stay on the ice for more than 30 minutes. Change From: 5. Centrifuge the tube in a refrigerated centrifuge (2-8°C) at 2000x g for 10 minutes and carefully transfer the plasma into a new storage tube or container.		

	To: 5. Centrifuge the tube at 2000x g for 10 minutes and carefully transfer the plasma into a new storage tube or container. 7. REAGENTS AND EQUIPMENT NEEDED BUT NOT PROVIDED Change From: 10. Refrigerated centrifuge (2-8°C) capable of 2000x g. To: 10. Centrifuge capable of 2000x g 11. ASSAY PROCEDURE Addition 9. Return leftover specimens to frozen storage at ≤ -20°C. Build: v1.5D BASE: v3.0
--	--

17. GENERAL INFORMATION

	Diagnostics Biochem Canada (DBC) Inc. 384 Neptune Crescent London, Ontario, Canada N6M 1A1 Tel: (519) 681-8731 Fax: (519) 681-8734 e-mail: dbc@dbc-labs.com www.dbc-labs.com
---	---

Product Complaints

In the case of product complaints, the user shall submit in writing to the distributor or manufacturer a description of the complaint and provide accompanying data and/or information.

















Warranty

DBC guarantees that the product is free of defects and will perform within the product specifications when the product is used prior to the expiration date, according to the intended purpose and use, and according to the instructions for use provided with the product. Any deviations from the intended purpose and use, instructions for use, modifications to kit components or use beyond the expiration date will invalidate any warranty claims.

Limitation of Liability

DBC liability in all circumstances whether in tort (including negligence) or at common law, and for any damage or loss, including but not limited to loss of profit and loss of sales, suffered whether direct, indirect, consequential, incidental or special is limited to the purchase price of the product(s) in question.

Symbols / Symbole / Symboles / Símbolos / Simboli / Símbolos / Σύμβολα

	Cat.-No.: / Kat.-Nr.: / No.- Cat.: / Cat.-No.: / N.-Cat.: / N.º Cat.: / Αριθμός-Κατ.:
	Lot-No.: / Chargen-Bez.: / No. Lot: / Lot-No.: / Lotto n.: / Lote N.º: / Αριθμός -Παραγωγή:
	Use by: / Verwendbar bis: / Utiliser à: / Usado por: / Da utilizzare entro:/ Usar até: / Χρησιμοποιείται από:
	No. of Tests: / Kitgröße: / Nb. de Tests: / No. de Determ.: / Quantità dei tests: / N.º de Testes: / Αριθμός εξετάσεων:
	Concentrate / Konzentrat / Concentré / Concentrar / Concentrato / Concentrado / Συμπύκνωμα
	Lyophilized / Lyophilisat / Lyophilisé / Liofilizado / Liofilizzato / Liofilizado / Λυοφιλοποιημένο
	In Vitro Diagnostic Medical Device / In-vitro-Diagnostikum / Appareil Médical pour Diagnostics In Vitro / Dispositivo Médico para Diagnóstico In Vitro / Dispositivo Medico Diagnostico In vitro / Equipamento Médico de Diagnóstico In Vitro / Ιατρική συσκευή για In-Vitro Διάγνωση
	Contains biological material of human origin / Enthält biologisches Material menschlichen Ursprungs / Contient une substance biologique d'origine humaine / Contiene material biológico de origen humano / Contiene materiale biologico di origine umana / Contém material biológico de origem humana / Περιέχει βιολογικό υλικό ανθρώπινης προέλευσης
	Contains biological material of animal origin / Enthält biologisches Material tierischen Ursprungs / Contient une substance biologique d'origine animale / Contiene material biológico de origen animal / Contiene materiale biologico di origine animale / Contém material biológico de origem animal / Περιέχει βιολογικό υλικό ζωικής προέλευσης
	Unique Device Identification / Eindeutige Geräteerkennung / Identifiant de dispositif unique / Identificación única de producto / Identificatore univoco del dispositivo / Identificador de dispositivo único / Μοναδικός αναγνωριστικός κωδικός προϊόντος
	Read instructions before use / Arbeitsanleitung lesen / Lire la fiche technique avant emploi / Lea las instrucciones antes de usar / Leggere le istruzioni prima dell'uso / Ler as instruções antes de usar / Διαβάστε τις οδηγίες πριν την χρήση
	Keep away from heat or direct sun light / Vor Hitze und direkter Sonneneinstrahlung schützen / Garder à l'abri de la chaleur et de toute exposition lumineuse / Manténgase alejado del calor o la luz solar directa / Non esporre ai raggi solari / Manter longe do calor ou luz solar directa / Να φυλάσσεται μακριά από θερμότητα και άμεση επαφή με το φως του ηλίου
	Store at: / Lagern bei: / Stocker à: / Almacene a: / Armazena a: / Conservare a: / Armazena em: / Αποθήκευση στους:
	Store at: 2 - 8°C / Lagern bei: 2 - 8°C / Stocker à: 2 - 8°C / Almacene a: 2 - 8°C / Armazena a: 2 - 8°C / Conservare a: 2-8°C / Armazena em: 2-8°C / Αποθήκευση στους: 2-8°C
	Manufacturer: / Hersteller: / Fabricant: / Productor: / Fabricante: / Fabbricante: / Παραγωγός:
	Distributor: / Distributor: / Distributeur: / Distributor: / Distributore: / Distribuidor: / Διανομέας:
	Caution! / Vorsicht! / Attention! / ¡Precaución! / Attenzione! / Cuidado! / Προσοχή!
	Symbols of the kit components see MATERIALS SUPPLIED. Die Symbole der Komponenten sind im Kapitel KOMPONENTEN DES KITS beschrieben. Voir MATERIEL FOURNI pour les symboles des composants du kit. Símbolos de los componentes del juego de reactivos, vea MATERIALES SUMINISTRADOS. Per i simboli dei componenti del kit si veda COMPONENTI DEL KIT. Para símbolos dos componentes do kit ver MATERIAIS FORNECIDOS. Για τα σύμβολα των συστατικών του κιτ συμβουλευτείτε το ΠΑΡΕΧΟΜΕΝΑ ΥΛΙΚΑ.

Generic table, not all symbols are present in the product

COMPLAINTS: Complaints may be submitted initially written or vocal. Subsequently they need to be filed including the test performance and results in writing in case of analytical reasons.

WARRANTY: The product is warranted to be free from material defects within the specific shelf life and to comply with product specifications delivered with the product. The product must be used according to the Intended use, all instructions given in the instructions for use and within the product specific shelf life. Any modification of the test procedure or exchange or mixing of components of different lots could negatively affect the results. These cases invalidate any claim for replacement.

LIMITATION OF LIABILITY: IN ALL CIRCUMSTANCES THE EXTENT OF MANUFACTURER'S LIABILITY IS LIMITED TO THE PURCHASE PRICE OF THE KIT(S) IN QUESTION. IN NO EVENT SHALL MANUFACTURER BE LIABLE FOR ANY INCIDENTAL OR CONSEQUENTIAL DAMAGES, INCLUDING DAMAGES FOR LOST PROFITS, LOST SALES, INJURY TO PERSON OR PROPERTY OR ANY OTHER INCIDENTAL OR CONSEQUENTIAL LOSS.

The labelling of hazardous substances is according to European directive.

For further country-specific classifications, please refer to the corresponding safety data sheet.



IBL International GmbH

Flughafenstrasse 52a
22335 Hamburg, Germany

Phone: +49 (0)40-53 28 91-0
Fax: +49 (0)40-53 28 91-11

IBL@tecan.com
www.tecan.com/ibl

Always there for you