

# Galectin-3 ELISA

Enzyme immunoassay for the quantitative determination of human galectin-3 in serum, plasma, cell lysate and cell culture supernatant

**REF**

**JP27755**



**12 x 8**

For illustrative purposes only.

To perform the assay the instructions for use provided with the kit have to be used.

Distributed by:

## Human Galectin-3 Assay Kit - IBL

### INTRODUCTION

Galectin is widely distributed in nematodes, insects, and porifers, as well as vertebrates, and it has also been found to be present in true fungi. Galectin does not just occur in the cytoplasm, it is also present in the nucleus, on the cell surface, in the extracellular matrix, etc., and it is thought to be involved in many biological phenomena, including development, differentiation, morphogenesis, tumor metastasis, cell death, and RNA splicing.

Galectin-3 is a  $\beta$ -galactoside-binding protein that has been named IgE-binding protein, CBP35, CBP30, Mac-2, L-29, L-31, L-34, etc., and structurally it is a chimera-type lectin composed of a sugar-chain-binding domain (galectin domain) and a non-lectin domain.

Its biological function is still uncertain, but many studies that should elucidate its function have been performed, and as a result participation of galectin-3 has been demonstrated in the biological phenomena of cell growth, adhesion, metastasis, and apoptosis. For example, a positive correlation has been shown between galectin-3 expression and the degree of malignant transformation in certain types of cell lines. A positive correlation has also recently been shown between galectin-3 expression and degree of malignancy in certain types of malignant tumors, and measurement of galectin-3 is expected to possibly serve as an index of degree of tumor malignancy.

### PRINCIPLE

This kit is a solid phase sandwich ELISA using 2 kinds of high specific antibodies. Tetra Methyl Benzidine (TMB) is used as coloring agent (Chromogen). The strength of coloring is in proportion to the quantities of human Galectin-3.

### MEASUREMENT RANGE

117.19 ~ 7,500 pg/mL

### INTENDED USE

- It enables measurement of Human galectin-3 in lysates of human cell cultures and clinical specimens (e.g., fine-needle aspiration cytology specimens of the thyroid gland).  
(Actual example 1)  
Appropriately dilute culture supernatant with "4, EIA buffer" in the kit, and use as the test specimen.  
(Actual example 2)  
Add 500  $\mu$ L of TNE buffer (10 mM Tris pH8.0, 1% NP-40, 0.15M NaCl, 1 mM EDTA) or IBL Code No.19022, IBLysis- I (Lysate buffer) to culture cells (rough guide:  $1 \times 10^5$ – $1 \times 10^7$  cells) or the clinical specimen, and after thoroughly mixing with a Vortex or by pipetting, mix by rotation at 4°C for 30 minutes. After the mixing has been completed, centrifuge at 10,000 rpm for 10 minutes, appropriately dilute (about 5–10 fold) the supernatant with "4, EIA buffer" in the kit, and use to make the measurements.
- To determine Human galectin-3 as a proportion of total protein, it is recommended to measure total protein after solubilizing it.  
The Lowry method is recommended for measuring total protein. (Lowry method [DC protein assay], BIO-RAD).
- When measuring cells, it is recommended that the number of cells be counted whenever possible.
- When making measurements of Human galectin-3 in human serum or plasma, appropriately dilute (about 4-10 fold) with "4, EIA buffer" in the kit, and use as the test specimen.

### KIT COMPONENT

1	Precoated plate	: Anti- Human Galectin-3 (50A3) Mouse IgG MoAb	96Well x 1
2	Labeled antibody Conc.	: (30X) HRP conjugated Anti- Human Galectin-3 (87B5) Mouse IgG MoAb	0.4mL x 1
3	Standard	: Recombinant Human Galectin-3	0.5mL x 2
4	EIA buffer*		30mL x 1
5	Solution for Labeled antibody*		12mL x 1
6	Chromogen	: TMB solution	15mL x 1
7	Stop solution*		12mL x 1
8	Wash buffer Conc.*		50mL x 1

### OPERATION MANUAL

#### 1. Materials needed but not supplied

- Plate reader (450nm)
- Graduated cylinder and beaker
- Refrigerator (as 4°C)
- Incubator (37°C  $\pm$  1°C)
- Tube for dilution of Standard
- Disposable test tube for "2, Labeled antibody Conc." and "6, Chromogen"
- Micropipette and tip
- Deionized water
- Graph paper (log/log)
- Paper towel
- Washing bottle for precoated plate


#### 2. Preparation

- 1) Preparation of wash buffer  
"8, Wash buffer Conc." is a concentrated (X40) buffer. The temperature of "8, Wash buffer Conc." shall be adjusted to room temperature and then, mix it gently and completely before use. Dilute 50mL of "8, Wash buffer Conc." with 1,950mL of deionized water and mix it. This is the wash buffer for use. This prepared wash buffer shall be stored in refrigerator and used within 2 weeks after dilution.
- 2) Preparation of Labeled antibody  
"2, Labeled antibody Conc." is a concentrated (X30). Dilute "2, Labeled antibody Conc." with "5, Solution for Labeled antibody" in 30 times according to required quantity into a disposable test tube. Use this resulting solution as Labeled antibody.  
Example)  
In case you use one slit (8 well), the required quantity of Labeled antibody is 800  $\mu$  L. (Dilute 30  $\mu$  L of "2, Labeled antibody Conc." with 870  $\mu$  L of "5, Solution for Labeled antibody" and mix it. And use the resulting solution by 100  $\mu$  L in each well.)  
This operation should be done just before the application of Labeled antibody.  
The remaining "2, Labeled antibody Conc." should be stored at 4°C in firmly sealed vial.
- 3) Preparation of Standard  
Put just 0.5 mL of deionized water into the vial of "3, Standard" and mix it gently and completely. This solution is 15,000 pg/mL Human Galectin-3 standard.

- 4) Dilution of Standard  
Prepare 8 tubes for dilution of "3, Standard". Put 230  $\mu$  L each of "4, EIA buffer" into the tube.  
Specify the following concentration of each tube.

Tube-1	7,500 pg/mL
Tube-2	3,750 pg/mL
Tube-3	1,875 pg/mL
Tube-4	937.5 pg/mL
Tube-5	468.75 pg/mL
Tube-6	234.38 pg/mL
Tube-7	117.19 pg/mL
Tube-8	0 pg/mL (Test Sample Blank)

Put 230  $\mu$  L of Standard solution into tube-1 and mix it gently. Then, put 230  $\mu$  L of tube-1 mixture into tube-2. Dilute two times standard solution in series to set up 7 points of diluted standard between 7,500 pg/mL and 117.19 pg/mL. Tube-8 is the test sample blank as 0 pg/mL.  
See following picture.

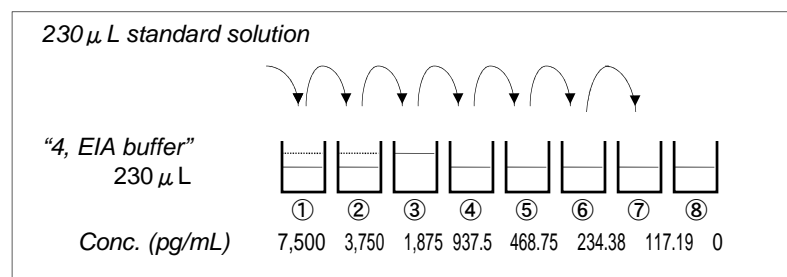

- 5) Dilution of test sample  
Test sample may be diluted with "4, EIA buffer" if the need arises.  
If the concentration of human Galectin-3 in samples may not be estimated in advance, the pre-assay with several different dilutions will be recommended to determine the proper dilution of samples.

### 3. Measurement procedure

All reagents shall be brought to room temperature approximately 30 minutes before use. Then mix it gently and completely before use. Confirm no change in quality of the reagents. Standard curve shall be prepared simultaneously with the measurement of test samples.

Reagents	Test Sample	Standard	Test Sample Blank	Reagent Blank
	Test sample 100 $\mu$ L	Diluted standard (Tube 1~7) 100 $\mu$ L	EIA buffer (Tube-8) 100 $\mu$ L	EIA buffer 100 $\mu$ L
Incubation for 1 hour at 37°C with plate lid				
4 times (wash buffer more than 350 $\mu$ L)*				
Labeled Antibody	100 $\mu$ L	100 $\mu$ L	100 $\mu$ L	-
Incubation for 30 minutes at 4°C with plate lid				
5 times (wash buffer more than 350 $\mu$ L)*				
Chromogen	100 $\mu$ L	100 $\mu$ L	100 $\mu$ L	100 $\mu$ L
Incubation for 30 minutes at room temperature (shielded)				
Stop solution	100 $\mu$ L	100 $\mu$ L	100 $\mu$ L	100 $\mu$ L
Read the plate at 450nm against a Reagent Blank within 30 minutes after application of Stop solution.				

- 1) Determine wells for reagent blank. Put 100  $\mu$  L each of "4, EIA buffer" into the wells.
- 2) Determine wells for test sample blank, test sample and diluted standard. Then, put 100  $\mu$  L each of test sample blank (tube-8), test sample and dilutions of standard (tube-1~7) into the appropriate wells.
- 3) Incubate the precoated plate for 1 hour at 37°C after covering it with plate lid.
- 4) Wash the plate with the prepared wash buffer and remove all liquid.\*
- 5) Pipette 100  $\mu$  L of labeled antibody solution into the wells of test samples, diluted standard and test sample blank.
- 6) Incubate the precoated plate for 30 minutes at 4°C after covering it with plate lid.
- 7) Wash the plate with the prepared wash buffer and remove all liquid.\*
- 8) "6, Chromogen" should be taken the required quantity into a disposable test tube. Then, pipette 100  $\mu$  L from the test tube into the wells. Please avoid to return the rest of test tube into "6, Chromogen" bottle due to avoid to cause of contamination.
- 9) Incubate the precoated plate for 30 minutes at room temperature in the dark. The liquid will turn blue by the addition of "6, Chromogen".
- 10) Pipette 100  $\mu$  L of "7, Stop solution" into the wells. Mix the liquid by tapping the side of precoated plate. The liquid will turn yellow by the addition of "7, Stop solution".
- 11) Remove any dirt or drop of water on the bottom of the precoated plate and confirm there is no bubble on the surface of the liquid. Then, run the plate reader and conduct measurement at 450nm.  
The measurement shall be done within 30 minutes after the addition of "7, Stop solution".

### SPECIAL ATTENTION

- 1) Test samples should be measured soon after the collection. In case of the storage of test samples, they should be stored under frozen conditions and do not repeat freeze/thaw cycles. Thaw the test samples at low temperature and mix them completely before measurement.
- 2) Test samples should be diluted with "4, EIA buffer", if the need arises.
- 3) The measurement of test samples and standard in duplicate is recommended.


- 4) Use test samples in neutral pH range. The contaminations of organic solvent may affect the measurement.
- 5) Use only wash buffer contained in this kit for washing the precoated plate. Insufficient washing may lead to the failure in measurement.
- 6) Remove the wash buffer completely by tapping the precoated plate on paper towel. Do not wipe wells with paper towel.
- 7) "6, Chromogen" should be stored in the dark due to its sensitivity against light. "6, Chromogen" should be avoided contact with metals.
- 8) Measurement should be done within 30 minutes after addition of "7, Stop solution".

#### CALCULATION OF TEST RESULT

Subtract the absorbance of test sample blank from all data, including standards and unknown samples before plotting. Plot the subtracted absorbance of the standards against the standard concentration on log-log graph paper. Draw the best smooth curve through these points to construct the standard curve. Read the concentration for unknown samples from the standard curve.

Example of standard curve

Conc. (pg/mL)	Absorbance (450nm)
7,500	2.173
3,750	1.173
1,875	0.650
937.5	0.333
468.75	0.179
234.38	0.100
117.19	0.061
0 (Test Sample Blank)	0.023

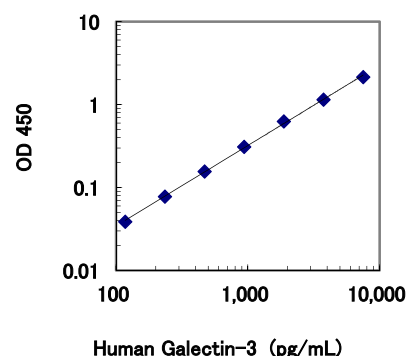

\* The typical standard curve is shown above. This curve can not be used to derive test results. Please run a standard curve for each assay.

#### PERFORMANCE CHARACTERISTICS

1. Titer Assay (Samples with standard added are used.)

Specimen	Titer (X)	Measurement Value (pg/mL)	Theoretical Value (pg/mL)	%
10% FCS added RPMI-1640	2	3,750.77	3,750.00	100.0
	4	1,881.83	1,875.00	100.4
	8	922.58	937.50	98.4
TNE buffer	2	3,680.67	3,750.00	98.2
	4	1,730.96	1,875.00	92.3
	8	826.46	937.50	88.2
Human Serum	2	6,260.26	6,061.15	103.3
	4	3,655.58	3,369.88	108.5
	8	2,038.87	1,868.52	109.1
	16	1,038.90	985.50	105.4
Human Plasma (EDTA)	4	5,692.99	5,685.24	100.1
	8	3,015.99	2,978.58	101.3
	16	1,785.43	1,627.85	109.7

2. Added Recovery Assay

Specimen	Theoretical Value (pg/mL)	Measurement Value (pg/mL)	%
10% FCS added RPMI-1640 (x2)	1,875.00	1,731.74	92.4
	937.50	867.50	92.5
	468.75	442.79	94.5
TNE buffer (x2)	937.50	802.47	85.6
	468.75	424.22	90.5
	234.38	214.01	91.3
Human Serum (x4)	2,937.96	3,215.32	109.4
	2,469.21	2,542.35	103.0
	2,234.84	2,204.54	98.6
Human Plasma (EDTA) (x4)	5,344.22	5,056.08	94.6
	4,875.47	4,601.78	94.4
	4,641.10	4,322.57	93.1

3. Intra – Assay

Measurement Value (pg/mL)	SD value	CV value (%)	n
5,363.51	216.66	4.0	24
1,229.51	49.54	4.0	24
267.41	14.83	5.5	24

4. Inter – Assay

Measurement Value (pg/mL)	SD value	CV value (%)	n
5,403.15	253.28	4.7	32
1,247.61	92.79	7.4	32
275.73	24.20	8.8	32

5. Specificity

Compound	Cross Reactivity
Human Galectin-3	100.0%
Human Galectin-1	≤0.1%
Human Galectin-4	0.21%
Mouse Galectin-3	≤0.1%

6. Sensitivity

43.95 pg/mL

The sensitivity for this kit was determined using the guidelines under the National Committee for Clinical Laboratory Standards (NCCLS) Evaluation Protocols. (National Committee for Clinical Laboratory Standards Evaluation Protocols, SC1, (1989) Villanova, PA: NCCLS.)

#### PRECAUTION FOR INTENDED USE AND/OR HANDLING

1. All reagents should be stored at 2~8°C. All reagents shall be brought to room temperature approximately 30 minutes before use.
2. "3, Standard" is lyophilized products. Be careful to open this vial.
3. "7, Stop solution" is a strong acid substance. Therefore, be careful not to contact your skin and clothes with "7, Stop solution" and pay attention to the disposal of "7, Stop solution".
4. Dispose used materials after rinsing them with large quantity of water.
5. The precipitation may grow in "2, Labeled antibody Conc.", however, there is no problem in the performance.
6. Wash hands after handling reagents.
7. Do not mix the reagents with the reagents from different lot or different kit.
8. Do not use the reagents expired.
9. This kit is for research purpose only. Do not use for clinical diagnosis.

#### STORAGE AND THE TERM OF VALIDITY

Storage Condition : 2 - 8 °C  
The expiry date is specified on outer box.

#### RELATED PRODUCTS

Code No.	Name	Volume
19022	IBLysis- I (Lysate buffer)	50×0.5 mL
		50 mL

#### REFERENCE

1. Ochieng J, Platt D, Tait L, Hogan V, Raz T, Carmi P, Raz A. Structure-function relationship of a recombinant human galactoside-binding protein. *Biochemistry*. 1993 Apr 27;32(16):4455-60.
2. Liu FT, Patterson RJ, Wang JL. Intracellular functions of galectins. *Biochim Biophys Acta*. 2002 Sep 19;1572(2-3):263-73.
3. Yang RY, Liu FT. Galectins in cell growth and apoptosis. *Cell Mol Life Sci*. 2003 Feb;60(2):267-76.
4. van den Brûle F, Califice S, Castronovo V. Expression of galectins in cancer: a critical review. *Glycoconj J*. 2004;19(7-9):537-42.
5. Takenaka Y, Fukumori T, Raz A. Galectin-3 and metastasis. *Glycoconj J*. 2004;19(7-9):543-9.
6. Inohara H, Segawa T, Miyauchi A, Yoshii T, Nakahara S, Raz A, Maeda M, Miyoshi E, Kinoshita N, Yoshida H, Furukawa M, Takenaka Y, Takamura Y, Ito Y, Taniguchi N. Cytoplasmic and serum galectin-3 in diagnosis of thyroid malignancies. *Biochem Biophys Res Commun*. 2008 Nov 21;376(3):605-10.













#### CONTACT DETAILS

Immuno-Biological Laboratories Co., Ltd.  
1091-1 Naka, Fujioka-Shi, Gunma 375-0005  
TEL : 0274-22-2889  
FAX : 0274-23-6055

Version 3.

January 2017 \*

# Symbols / Symbole / Symbôles / Símbolos / Símbolos / Σύμβολα

	Cat.-No.: / Kat.-Nr.: / No.- Cat.: / Cat.-No.: / N.º Cat.: / N.-Cat.: / Αριθμός-Κατ.:
	Lot-No.: / Chargen-Bez.: / No. Lot: / Lot-No.: / Lote N.º: / Lotto n.: / Αριθμός -Παραγωγή:
	Use by: / Verwendbar bis: / Utiliser à: / Usado por: / Usar até: / Da utilizzare entro: / Χρησιμοποιείται από:
	No. of Tests: / Kitgröße: / Nb. de Tests: / No. de Determ.: / N.º de Testes: / Quantità dei tests: / Αριθμός εξετάσεων:
	Concentrate / Konzentrat / Concentré / Concentrar / Concentrado / Concentrato / Συμπύκνωμα
	Lyophilized / Lyophilisat / Lyophilisé / Liofilizado / Liofilizado / Liofilizzato / Λυοφιλιασμένο
	In Vitro Diagnostic Medical Device. / In-vitro-Diagnostikum. / Appareil Médical pour Diagnostics In Vitro. / Dispositivo Médico para Diagnóstico In Vitro. / Equipamento Médico de Diagnóstico In Vitro. / Dispositivo Medico Diagnostico In vitro. / Ιατρική συσκευή για In-Vitro Διάγνωση.
	Evaluation kit. / Nur für Leistungsbewertungszwecke. / Kit pour évaluation. / Juego de Reactivos para Evaluació. / Kit de avaliação. / Kit di evaluazione. / Κιτ Αξιολόγησης.
	Read instructions before use. / Arbeitsanleitung lesen. / Lire la fiche technique avant emploi. / Lea las instrucciones antes de usar. / Ler as instruções antes de usar. / Leggere le istruzioni prima dell'uso. / Διαβάστε τις οδηγίες πριν την χρήση.
	Keep away from heat or direct sun light. / Vor Hitze und direkter Sonneneinstrahlung schützen. / Garder à l'abri de la chaleur et de toute exposition lumineuse. / Manténgase alejado del calor o la luz solar directa. / Manter longe do calor ou luz solar directa. / Non esporre ai raggi solari. / Να φυλάσσεται μακριά από θερμότητα και άμεση επαφή με το φως του ηλίου.
	Store at: / Lagern bei: / Stocker à: / Almacene a: / Armazemar a: / Conservare a: / Αποθήκευση στους:
	Manufacturer: / Hersteller: / Fabricant: / Productor: / Fabricante: / Fabbicante: / Παραγωγός:
	Caution! / Vorsicht! / Attention! / ¡Precaución! / Cuidado! / Attenzione! / Προσοχή!
<p>Symbols of the kit components see MATERIALS SUPPLIED.  Die Symbole der Komponenten sind im Kapitel KOMPONENTEN DES KITS beschrieben.  Voir MATERIEL FOURNI pour les symbôles des composants du kit.  Símbolos de los componentes del juego de reactivos, vea MATERIALES SUMINISTRADOS.  Para símbolos dos componentes do kit ver MATERIAIS FORNECIDOS.  Per i simboli dei componenti del kit si veda COMPONENTI DEL KIT.  Για τα σύμβολα των συστατικών του κιτ συμβουλευτείτε το ΠΑΡΕΧΟΜΕΝΑ ΥΛΙΚΑ.</p>	

COMPLAINTS: Complaints may be submitted initially written or vocal. Subsequently they need to be filed including the test performance and results in writing in case of analytical reasons.

WARRANTY: The product is warranted to be free from material defects within the specific shelf life and to comply with product specifications delivered with the product. The product must be used according to the Intended use, all instructions given in the instructions for use and within the product specific shelf life. Any modification of the test procedure or exchange or mixing of components of different lots could negatively affect the results. These cases invalidate any claim for replacement.

LIMITATION OF LIABILITY: IN ALL CIRCUMSTANCES THE EXTENT OF MANUFACTURER'S LIABILITY IS LIMITED TO THE PURCHASE PRICE OF THE KIT(S) IN QUESTION. IN NO EVENT SHALL MANUFACTURER BE LIABLE FOR ANY INCIDENTAL OR CONSEQUENTIAL DAMAGES, INCLUDING DAMAGES FOR LOST PROFITS, LOST SALES, INJURY TO PERSON OR PROPERTY OR ANY OTHER INCIDENTAL OR CONSEQUENTIAL LOSS.

**IBL International GmbH**  
Flughafenstr. 52A, 22335 Hamburg, Germany

Tel.: + 49 (0) 40 532891 -0 Fax: -11  
E-MAIL: IBL@IBL-International.com  
WEB: <http://www.IBL-International.com>