

## Instructions for Use

# GLP-1 (active) ELISA

Enzyme immunoassay for the quantitative determination of active Glucagon-Like Peptide-1 (GLP-1(7-36) and GLP-1(7-37)) in EDTA plasma.

**REF** **JP27784**

 **12x8**

For illustrative purposes only.

To perform the assay the instructions for use provided with the kit have to be used.

Distributed by: **IBL International GmbH**

Flughafenstrasse 52a

D-22335 Hamburg, Germany

Phone: +49 (0)40-53 28 91-0

Fax: +49 (0)40-53 28 91-11

IBL@tecan.com

www.tecan.com/ibl

**Always there for you**



Code No. 27784

## GLP-1, Active form Assay Kit - IBL

### INTRODUCTION

Incretins are a group of gastrointestinal hormones that cause an increase in the amount of insulin released from the beta cells of the islets of Langerhans after eating. They also inhibit glucagon release from the alpha cells of the islets of Langerhans. As a result, they slow the rate of absorption of nutrients into the blood stream by reducing gastric emptying and may directly reduce food intake.

The two main candidate molecules that fulfill criteria for an incretin are glucagon-like peptide-1 (GLP-1) and Gastric inhibitory peptide (or glucose-dependent insulinotropic polypeptide or GIP).

The human *proglucagon* gene was cloned in 1983, and the human proglucagon sequence was subsequently deduced. After that, it was found that the specific sequence of GLP-1 has insulinotropic effect: GLP-1 (7-36) amide. Now, GLP-1 (7-36) amide and GLP-1 (7-37) are known as active forms of GLP-1. They are rapidly inactivated to GLP-1 (9-36) amide and GLP-1 (9-37) by DPP-IV within a few moments in blood. This ELISA kit can measure active forms of GLP-1 (GLP-1 (7-36) amide and GLP-1 (7-37)) specifically.

### PRINCIPLE

This kit is a solid phase sandwich ELISA using 2 kinds of highly specific antibodies. Tetra Methyl Benzidine (TMB) is used as a coloring agent (Chromogen). The strength of coloring is proportional to the quantities of active form of GLP-1.

### MEASUREMENT RANGE

1.25 - 80 pmol/L

(4.1 - 263.8 pg/mL of GLP-1 (7-36) amide (as molecular weight is 3297.6))

### INTENDED USE

For research use only, not for use in diagnostic procedures.

This IBL's assay kit is capable for the quantitative determination active form of GLP-1 (GLP-1 (7-36) amide and GLP-1 (7-37)) in EDTA-plasma.

DPP-IV inhibitor has to be added when collecting samples, or use purpose-made blood collection tubes in order to preserve GLP-1 active form. (eg. BD™ Blood Collection System for Preservation of Plasma GLP-1, GIP, Glucagon and Ghrelin, BD Diagnostics)

### KIT COMPONENT

1	Precoated plate : Anti-GLP-1 Rabbit IgG Affinity Purify	96Well x 1
2	Labeled antibody Conc. : (30X) HRP conjugated Anti-GLP-1 (34B1) Mouse IgG MoAb Fab' Affinity Purify	0.4mL x 1
3	Standard : GLP-1 (7-36) amide	0.5mL x 2
4	EIA buffer	30mL x 1
5	Solution for Labeled antibody	12mL x 1
6	Chromogen : TMB solution	15mL x 1
7	Stop solution	12mL x 1
8	Wash buffer Conc.	50mL x 1

### OPERATION MANUAL

#### 1. Materials needed but not supplied

- Plate reader (450nm)
- Graduated cylinder and beaker
- Refrigerator (as 4°C)
- Paper towel
- Incubator (37°C ± 1°C)
- Washing bottle for precoated plate
- Disposable test tube for "2, Labeled antibody Conc." and "6, Chromogen"
- Micropipette and tip
- Deionized water
- Graph paper (log/log)
- Tube for dilution of Standard

#### 2. Preparation

##### 1) Preparation of wash buffer

"8, Wash buffer Conc." is a concentrated (40X) buffer. Adjust the temperature of "8, Washing buffer Conc." to room temperature and then, mix it gently and completely before use. Dilute 50 mL of "8, Wash buffer Conc." with 1,950 mL of deionized water and mix it. This is the wash buffer for use. This prepared wash buffer shall be stored in refrigerator and used within 2 weeks after dilution.

##### 2) Preparation of Labeled antibody

"2, Labeled antibody Conc." is a concentrated (30X). Dilute "2, Labeled antibody Conc." with "5, Solution for Labeled antibody" in 30 times according to required quantity into a disposable test tube. Use this resulting solution as Labeled antibody.

Example)

In case you use one strip (8 well), the required quantity of Labeled antibody is 800 µL. (Dilute 30 µL of "2, Labeled antibody Conc." with 870 µL of "5, Solution for Labeled antibody" and mix it. And use the resulting solution by 100 µL in each well.)

This operation should be done just before the applying of Labeled antibody.

The remaining "2, Labeled antibody Conc." should be stored at 4°C in firmly sealed vial.

##### 3) Preparation of Standard

Put just 0.5 mL of deionized water into the vial of "3, Standard" and mix it gently and completely. This solution is 160 pmol/L GLP-1 (7-36) amide standard.

##### 4) Dilution of Standard

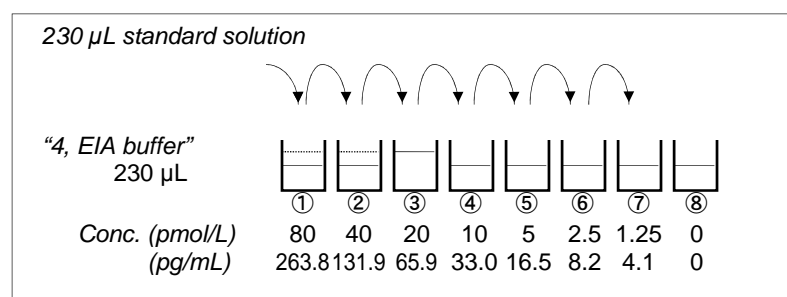
Prepare 8 tubes for dilution of "3, Standard". Put 230 µL each of "4, EIA buffer" into the tube.

Specify the following concentration of each tube."

Tube-1	80 pmol/L
Tube-2	40 pmol/L
Tube-3	20 pmol/L
Tube-4	10 pmol/L
Tube-5	5 pmol/L
Tube-6	2.5 pmol/L
Tube-7	1.25 pmol/L
Tube-8	0 pmol/L (Test Sample Blank)

Put 230 µL of Standard solution into tube-1 and mix it gently. Then, put 230 µL of tube-1 mixture into tube-2. Dilute two times standard solution in series to set up 7 points of diluted standard between 80 pmol/L and 1.25 pmol/L. Tube-8 is the test sample blank as 0 pmol/L.

See following picture.



#### 5) Dilution of test sample

Test samples should be diluted with "4, EIA buffer" as necessary.

If the concentration of active form GLP-1 in samples may not be estimated in advance, the pre-assay with several different dilutions will be recommended to determine the proper dilution of samples.

### 3. Measurement procedure

All reagents shall be brought to room temperature approximately 30 minutes before use. Then mix it gently and completely before use. Make sure of no change in quality of the reagents. Standard curve shall be prepared simultaneously with the measurement of test samples.

Reagents	Test Sample	Standard	Test Sample Blank	Reagent Blank
Test sample	100 µL	Diluted standard (Tube 1-7) 100 µL	EIA buffer (Tube-8) 100 µL	EIA buffer 100 µL
Incubation for 60 minutes at 37°C with plate lid				
4 times (wash buffer more than 350 µL)				
Labeled Antibody	100 µL	100 µL	100 µL	-
Incubation for 60 minutes at 4°C with plate lid				
5 times (wash buffer more than 350 µL)				
Chromogen	100 µL	100 µL	100 µL	100 µL
Incubation for 30 minutes at room temperature (shielded)				
Stop solution	100 µL	100 µL	100 µL	100 µL
Read the plate at 450nm against a Reagent Blank within 30 minutes after addition of Stop solution.				

- 1) Determine wells for reagent blank. Put 100 µL each of "4, EIA buffer" into the wells.
- 2) Determine wells for test sample blank, test sample and diluted standard. Then, put 100 µL each of test sample blank (tube-8), test sample and dilutions of standard (tube-1-7) into the appropriate wells.
- 3) Incubate the precoated plate for 60 minutes at 37°C after covering it with plate lid.
- 4) Wash the plate with the prepared wash buffer and remove all liquid.
- 5) Pipette 100 µL of labeled antibody solution into the wells of test samples, diluted standard and test sample blank.
- 6) Incubate the precoated plate for 60 minutes at 4°C after covering it with plate lid.
- 7) Wash the plate with the prepared wash buffer and remove all liquid.
- 8) Take the required quantity of "6, Chromogen" into a disposable test tube. Then, pipette 100 µL from the test tube into every well. Please do not return the rest of used chromogen in the test tube into "6, Chromogen" bottle in order to avoid contamination.
- 9) Incubate the precoated plate for 30 minutes at room temperature in the dark. The solution of Chromogen will turn blue.
- 10) Add 100 µL of "7, Stop solution" to all wells. Mix the solution by tapping the side of precoated plate. The solution will turn yellow by addition of "7, Stop solution".
- 11) Remove any dirt or drop of water on the bottom of the precoated plate and confirm there is no bubble on the surface of the solution. Then, run the plate reader and conduct measurement at 450 nm against a reagent blank. The measurement shall be done within 30 minutes after addition of "7, Stop solution".

### SPECIAL ATTENTION

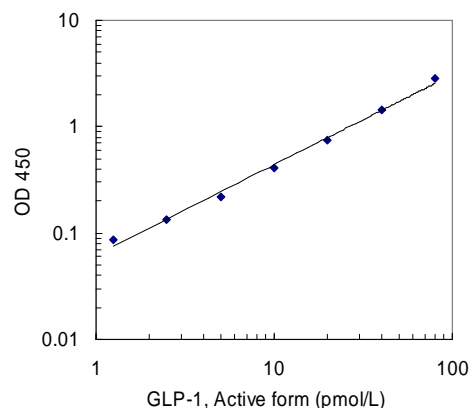
- 1) Test samples should be measured soon after collection. For the storage of test samples, store them frozen and do not repeat freeze/thaw cycles. Thaw the test samples at a low temperature and mix them completely before measurement.
- 2) Test samples should be diluted with "4, EIA buffer", as the need arises.
- 3) Duplicate measurement of test samples and standard is recommended.
- 4) Use test samples in neutral pH range. The contaminations of organic solvent may affect the measurement.
- 5) Use only wash buffer in this kit for washing the precoated plate. Insufficient or overdone washing may lead to the failure in measurement.
- 6) Remove the wash buffer completely by tapping the precoated plate on paper towel. Do not wipe wells with paper towel.
- 7) "6, Chromogen" should be stored in the dark due to its sensitivity against light. "6, Chromogen" should be avoided contact with metals.
- 8) Measurement should be done within 30 minutes after addition of "7, Stop solution".

**CALCULATION OF TEST RESULT**





Subtract the absorbance of test sample blank from all data, including standards and unknown samples before plotting. Plot the subtracted absorbance of the standards against the standard concentration on log-log graph paper. Draw the best smooth curve through these points to construct the standard curve. Read the concentration for unknown samples from the standard curve.

Example of standard curve

Conc. (pmol/L)	Absorbance (450nm)
80	2.883
40	1.499
20	0.809
10	0.469
5	0.275
2.5	0.193
1.25	0.144
0 (Test Sample Blank)	0.058



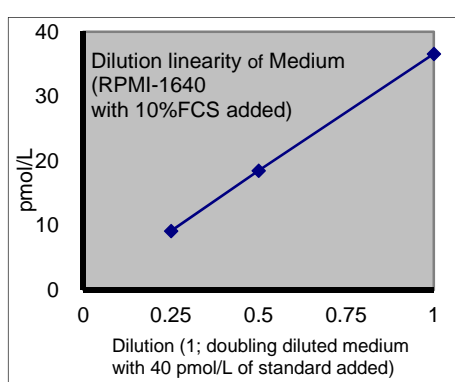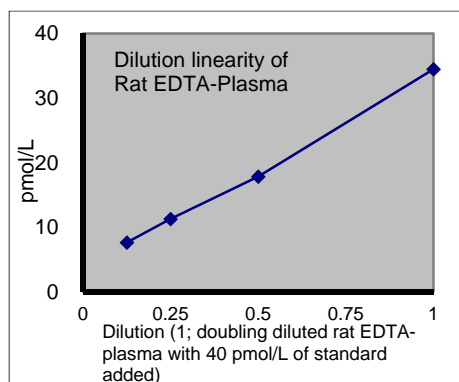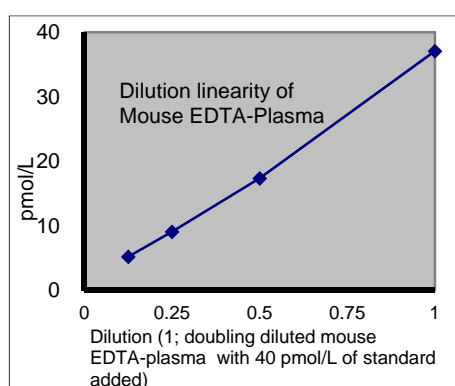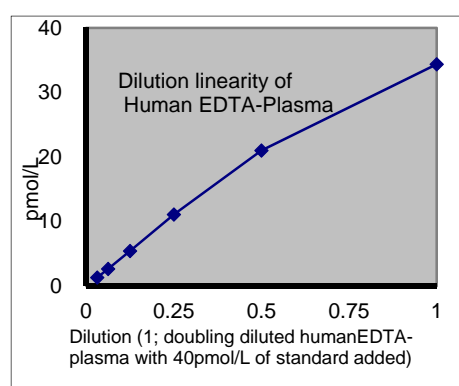\* The typical standard curve is shown above. This curve can not be used to derive test results. Please run a standard curve for each assay.

**PERFORMANCE CHARACTERISTICS**
**1. Dilution Linearity**


\*The plasma sample was collected by usual method with EDTA and added with DPP-IV inhibitor after separation.

**2. Added Recovery Assay**

Specimen	Theoretical Value (pmol/L)	Measurement Value (pmol/L)	%
*Human Plasma (EDTA) (x2)	41.40	33.93	82.0
	21.40	18.91	88.4
	11.40	9.96	87.4
*Mouse Plasma (EDTA) (BALB/c) (x2)	42.51	39.93	93.9
	22.51	20.93	93.0
	12.51	11.54	92.2
*Rat Plasma (EDTA) (SD) (x2)	21.24	17.75	83.6
	11.24	9.20	81.9
	6.24	5.19	83.2
10%FCS added RPMI-1640 (x2)	40.41	38.02	94.1
	20.41	20.33	99.6
	10.41	9.96	95.7

\*The plasma sample was collected by usual method with EDTA, and added with DPP-IV inhibitor after separation.

**3. Intra - Assay**

Measurement Value (pmol/L)	SD value	CV value (%)	n
41.56	2.26	5.4	24
11.38	0.51	4.5	24
2.43	0.13	5.5	24

**4. Inter - Assay**

Measurement Value (pmol/L)	SD value	CV value (%)	n
41.62	3.03	7.3	7
11.24	0.80	7.1	7
2.18	0.24	10.9	7

**5. Specificity**

Compound	Cross Reactivity
GLP-1 (7-36) amide	100 %
GLP-1 (7-37)	100 %
GLP-1 (1-37)	0.32 %
GLP-1 (9-36) amide	< 0.1 %
GLP-2	< 0.1 %
Glucagon	< 0.1 %
Human GIP	< 0.1 %
Mouse GIP	< 0.1 %

**6. Sensitivity**

0.10 pmol/L

The sensitivity for this kit was determined using the guidelines under the National Committee for Clinical Laboratory Standards (NCCLS) Evaluation Protocols. (National Committee for Clinical Laboratory Standards Evaluation Protocols, SC1, (1989) Villanova, PA: NCCLS.)

**PRECAUTION FOR INTENDED USE AND/OR HANDLING**

- All reagents should be stored at 2 - 8°C. All reagents shall be brought to room temperature approximately 30 minutes before use.
- "3, Standard" is lyophilized products. Be careful to open this vial.
- "7, Stop solution" is a strong acid substance. Therefore, be careful not to have your skin and clothes contact "7, Stop solution" and pay attention to the disposal of "7, Stop solution".
- Dispose used materials after rinsing them with large quantity of water.
- Precipitation may occur in "2, Labeled antibody Conc.", "4, EIA buffer" or "8, Wash buffer Conc.", however, there is no problem in the performance.
- Wash hands after handling reagents.
- Do not mix the reagents with the reagents from a different lot or kit.
- Do not use expired reagents.
- This kit is for research purpose only. Do not use for clinical diagnosis.

**STORAGE AND THE TERM OF VALIDITY**

Storage Condition : 2 - 8°C

The expiry date is specified on outer box.

Version 3.

August 2018 \*

Made in Japan.

**IBL Incretin-related Products:**

Code No.	Name	Volume
27203	Human GIP, Total Assay Kit - IBL	96 Well
27201	Human GIP, Active form Assay Kit - IBL	96 Well
27701*	Mouse GIP, Total (high sensitivity) Assay Kit - IBL	96 Well
27702*	Mouse GIP, Active form (high sensitivity) Assay Kit - IBL	96 Well
27703*	Rat GIP, Total (high sensitivity) Assay Kit - IBL	96 Well
27704*	Rat GIP, Active form (high sensitivity) Assay Kit - IBL	96 Well
27784	GLP-1, Active form Assay Kit - IBL	<b>96 Well</b>
27788	GLP-1(9-36/37) form Assay Kit - IBL	96 Well
27700	GLP-1, Active form (High sensitivity) Assay-IBL*	96 Well

# Symbols / Symbole / Symbôles / Símbolos / Símbolos / Σύμβολα

	Cat.-No.: / Kat.-Nr.: / No.- Cat.: / Cat.-No.: / N.º Cat.: / N.-Cat.: / Αριθμός-Κατ.:
	Lot-No.: / Chargen-Bez.: / No. Lot: / Lot-No.: / Lote N.º: / Lotto n.: / Αριθμός -Παραγωγή:
	Use by: / Verwendbar bis: / Utiliser à: / Usado por: / Usar até: / Da utilizzare entro: / Χρησιμοποιείται από:
	No. of Tests: / Kitgröße: / Nb. de Tests: / No. de Determ.: / N.º de Testes: / Quantità dei tests: / Αριθμός εξετάσεων:
	Concentrate / Konzentrat / Concentré / Concentrar / Concentrado / Concentrato / Συμπύκνωμα
	Lyophilized / Lyophilisat / Lyophilisé / Liofilizado / Liofilizado / Liofilizzato / Λυοφιλιασμένο
	In Vitro Diagnostic Medical Device. / In-vitro-Diagnostikum. / Appareil Médical pour Diagnostics In Vitro. / Dispositivo Médico para Diagnóstico In Vitro. / Equipamento Médico de Diagnóstico In Vitro. / Dispositivo Medico Diagnostico In vitro. / Ιατρική συσκευή για In-Vitro Διάγνωση.
	Evaluation kit. / Nur für Leistungsbewertungszwecke. / Kit pour évaluation. / Juego de Reactivos para Evaluació. / Kit de avaliação. / Kit di valutazione. / Κιτ Αξιολόγησης.
	Read instructions before use. / Arbeitsanleitung lesen. / Lire la fiche technique avant emploi. / Lea las instrucciones antes de usar. / Ler as instruções antes de usar. / Leggere le istruzioni prima dell'uso. / Διαβάστε τις οδηγίες πριν την χρήση.
	Keep away from heat or direct sun light. / Vor Hitze und direkter Sonneneinstrahlung schützen. / Garder à l'abri de la chaleur et de toute exposition lumineuse. / Manténgase alejado del calor o la luz solar directa. / Manter longe do calor ou luz solar directa. / Non esporre ai raggi solari. / Να φυλάσσεται μακριά από θερμότητα και άμεση επαφή με το φως του ηλίου.
	Store at: / Lagern bei: / Stocker à: / Almacene a: / Armazemar a: / Conservare a: / Αποθήκευση στους:
	Manufacturer: / Hersteller: / Fabricant: / Productor: / Fabricante: / Fabbicante: / Παραγωγός:
	Caution! / Vorsicht! / Attention! / ¡Precaución! / Cuidado! / Attenzione! / Προσοχή!
<p>Symbols of the kit components see MATERIALS SUPPLIED.</p> <p>Die Symbole der Komponenten sind im Kapitel KOMPONENTEN DES KITS beschrieben.</p> <p>Voir MATERIEL FOURNI pour les symbôles des composants du kit.</p> <p>Símbolos de los componentes del juego de reactivos, vea MATERIALES SUMINISTRADOS.</p> <p>Para símbolos dos componentes do kit ver MATERIAIS FORNECIDOS.</p> <p>Per i simboli dei componenti del kit si veda COMPONENTI DEL KIT.</p> <p>Για τα σύμβολα των συστατικών του κιτ συμβουλευτείτε το ΠΑΡΕΧΟΜΕΝΑ ΥΛΙΚΑ.</p>	

COMPLAINTS: Complaints may be submitted initially written or vocal. Subsequently they need to be filed including the test performance and results in writing in case of analytical reasons.

WARRANTY: The product is warranted to be free from material defects within the specific shelf life and to comply with product specifications delivered with the product. The product must be used according to the Intended use, all instructions given in the instructions for use and within the product specific shelf life. Any modification of the test procedure or exchange or mixing of components of different lots could negatively affect the results. These cases invalidate any claim for replacement.

LIMITATION OF LIABILITY: IN ALL CIRCUMSTANCES THE EXTENT OF MANUFACTURER'S LIABILITY IS LIMITED TO THE PURCHASE PRICE OF THE KIT(S) IN QUESTION. IN NO EVENT SHALL MANUFACTURER BE LIABLE FOR ANY INCIDENTAL OR CONSEQUENTIAL DAMAGES, INCLUDING DAMAGES FOR LOST PROFITS, LOST SALES, INJURY TO PERSON OR PROPERTY OR ANY OTHER INCIDENTAL OR CONSEQUENTIAL LOSS.

Distributed **IBL International GmbH**

by: Flughafenstrasse 52a  
D-22335 Hamburg, Germany

Phone: +49 (0)40-53 28 91-0  
Fax: +49 (0)40-53 28 91-11

IBL@tecan.com  
www.tecan.com/ibl

**Always there for you**

