


Instructions for use

beta 2-Glycoprotein 1 IgG ELISA

Enzyme immunoassay for the qualitative and quantitative determination of IgG antibodies against β 2-glycoprotein 1 in human serum or plasma (EDTA, citrate, heparin).

REF RE75051

 12x8

  2°C  8°C

EU: **IVD** 



IBL International GmbH
Flughafenstrasse 52a
D-22335 Hamburg, Germany

Always there for you



1. Introduction and background

The anti-phospholipid syndrome (APS) is a systemic autoimmune disorder which can comprise clinical conditions as venous and arterial thrombosis, thrombocytopenia, myocardial infarction, recurrent spontaneous abortion and neurological complications (1, 2, 3, 4). In addition to these clinical manifestations, the persistent presence of a unique collection of autoantibodies is what defines the syndrome. These autoantibodies target specific phospholipids and phospholipid-binding proteins.

Among the phospholipids, Cardiolipin (CL) is the most common one, negatively charged and acid. beta2-glycoprotein 1 (β 2-GP1; = apolipoprotein H) has been identified as natural and essential co-antigen for CL-autoantibodies (5, 6). Besides this diagnostic significance, these antibodies cause a hypercoagulable state, associated with a tendency towards thromboses (4, 7, 8), and are believed to be directly involved in the pathogenesis of APS (9, 10). The actual mechanism of this effect however remains elusive.

The present enzyme-linked immuno sorbent assay (ELISA) is intended for the quantitative or qualitative determination of IgG antibodies directed against β 2-GP1 in human serum or plasma (cf. section 7). The immobilised antigen is a highly purified preparation of human β 2-GP1. The test is fast (incubation time 30 - 30 - 30 minutes) and flexible (divisible solid phase, ready-to-use reagents). Six calibrators allow quantitative measurements; a negative and a positive control check the assay performance.

2. Warnings and precautions

The test kit is intended for in vitro diagnostic use only; not for internal or external use in humans or animals.

It must be executed by trained personnel staff.

Do not use reagents beyond their expiration dates.

Adherence to the protocol is strongly recommended.

The sample buffer, calibrators and controls contain Na-azide as antimicrobial agent. The wash buffer contains bromonitrodioxane and the conjugate methylisothiazolone / bromonitrodioxane as preservative. The substrate contains 3, 3', 5, 5'-tetramethylbenzidine (TMB) and hydrogen peroxide (H₂O₂). The stop solution, 0,2 M sulfuric acid (H₂SO₄), is acidic and corrosive.

The above mentioned reagents may be toxic if ingested. Follow routine precautions for handling hazardous chemicals. Avoid all body contact, wear gloves and eye protection. If one of the reagents comes into contact with skin or mucous membrane, wash thoroughly with water. Never pipette by mouth. Dispose in a manner complying with local/national regulations.

Na-Azide may react with lead and copper plumbing to form explosive metal azides. On disposal, flush with a large amount of water to prevent azide build-up.

The calibrators and controls contain components of human origin. They were tested for human immunodeficiency virus (HIV)-Ag, hepatitis B surface (HBs)-Ag and antibodies against HIV 1/2 and hepatitis C virus (HCV) and showed negative results; either in an FDA-approved or a CE-compliant test, according to European Directive 98/79/EC.

However, no test can guarantee that material of human origin is not actually infectious. The preparations should therefore be treated as potentially infectious and disposed of accordingly, as should the samples (and residues thereof); according to CDC (Center of Disease Control, Atlanta, USA) or other local / national guidelines on laboratory safety and decontamination.

3. Principle of the test

The wells of the solid phase are coated with β 2-GP1. On this surface, the following immunological reactions take place:

1st reaction: β 2-GP1-specific antibodies present in the sample bind to the immobilised antigen, forming the antigen-antibody complex. Then, non-bound sample components are washed away from the solid phase.

2nd reaction: A second antibody, directed at human IgG antibodies and conjugated with horse-radish peroxidase (HRP), is added. This conjugate binds to the complex. Then, excess conjugate is washed away from the solid phase.

3rd reaction: The enzyme-labelled complex converts a colourless substrate into a blue product. The degree of colour development reflects the concentration of β 2-GP1 IgG in the sample.

4. Contents of the kit

- a. **MTP Microtiter Plate**, coated with β 2-GP1 and hermetically packed in a foil laminate pouch together with a desiccant bag. The plate consists of 12 strips, each of which can be broken into 8 individual wells.
- b. **ENZCONJ IgG Enzyme Conjugate IgG**, 14 mL, ready-to-use, red coloured. Buffered solution containing stabilising protein, methylisothiazolone and bromonitrodioxane.
- c. **CAL A-F Calibrator A-F**, 2,0 mL each, 0 - 3,0 - 8,0 - 18 - 45 and 100 U β 2-GP1 IgG / mL, ready-to-use, gradually blue coloured. Contain TBS, BSA, Tween and Na-azide.
- d. **CONTROL - & CONTROL + Negative and Positive Control**, 2,0 mL each, ready-to-use, green and red coloured, respectively. Contain TBS, BSA, Tween and Na-azide.
- e. **SAMPLEDIL Sample Diluent**, 100 mL, ready-to-use, orange coloured. Contains Tris-buffered saline (TBS), bovine serum albumin (BSA), Tween and Na-azide.
- f. **TMB SUBS TMB Substrate Solution**, 14 mL, ready-to-use, colourless. Contains a buffered solution of TMB and H_2O_2 . Contained in a vial impermeable to light.
- g. **WASHBUF CONC Wash Buffer**, 100 mL, 10x-concentrate, blue coloured. Contains TBS, Tween and bromonitrodioxane. TBS, BSA, Tween and Na-azide.
- h. **STOP TMB Stop Solution** (0,2 M H_2SO_4), 14 mL, colourless, ready-to-use.
Caution: sulfuric acid is corrosive.
- i. Directions for use
- j. Lot-specific certificate of analysis

5. Materials required but not supplied

- a. Deionised or distilled water
- b. Graduated cylinder, 1000 mL
- c. Tubes for sample dilution (transfer tubes in the microwell plate format recommended)
- d. Pipettes for 10, 100 and 1000 μ L (1- and 8-channel pipettes recommended)
- e. Microwell plate washer (optional)
- f. Microwell plate photometer fitted with a 450 nm filter
- g. ELISA evaluation program (recommended)

6. Storage of the kit

Store kit at 2 - 8°C. It is stable up to the expiry date stated on the label of the box. Do not use kit beyond its expiry date.

7. Reagent and sample preparation / specimen requirements

Do not exchange or pool corresponding components from different kits, due to possibly different shipping or storage conditions. If the kit is to be used for several tests, only the currently needed amount of reagents should be withdrawn. It is **crucially important** that no cross-contamination between the reagents occurs. Use only clean pipettes and do **not pour back** residues into the original flasks.

- a. The solid phase must reach room temperature before opening the pouch. Remove the supernumerary microwells from the frame and immediately put them back into the pouch, together with the desiccant bag. Reseal the pouch hermetically and keep it refrigerated for future use.
- b. Dilute the wash buffer 10x-concentrate (100 mL, blue) with 900 mL deionised water. Mix thoroughly. The diluted buffer is stable for several weeks if stored refrigerated (2 - 8°C).
- c. Preparation of the samples: handle patient specimens as potentially infectious agents. Besides serum, EDTA-, citrate- or heparin-treated plasma is suitable sample material as well.

Specimen requirements: highly lipemic, haemolysed or microbially contaminated samples may cause erroneous results and should be avoided.

Prepare samples using normal laboratory techniques. Turbid samples must first be clarified (centrifuged). The clarified or clear samples are mixed and then diluted 1/100, e.g. 10 µL serum or plasma + 990 µL sample buffer. Also mix the dilution.

For rapid dispensing during the assay procedure, preparation of the calibrators, controls and samples in microwell transfer tubes is recommended. This allows the operation of an 8-channel pipette during the assay procedure.

If samples are not assayed immediately, they should be stored at 2 - 8°C and assayed within 3 days. For longer storage, -20°C or lower temperatures are recommended. Repeated freezing and thawing of samples should be avoided. Thawed samples must be mixed prior to diluting.

8. Assay procedure

Before starting the assay, all components of the kit must have reached room temperature (23 ± 3°C).

To achieve best results, i.e. the maximum ratio between specific and background signal, **careful washing** is essential (steps a, c and e). It is **crucially important to remove the wash solution completely**. For that purpose, tap the plate firmly on several layers of absorbent tissue. Automated washers must be verified according to results obtained by manual washing.

- a. Immediately prior to use, wash the solid phase once: fill wells with 350 µL wash buffer each, let soak for about 10 seconds in the wells and remove.
- b. Dispense the calibrators (2,0 mL each, ready-to-use, gradually blue), controls (2,0 mL each, ready-to-use, green and red) and the diluted samples rapidly into the microwells; 100 µL per well. Duplicate measurements are recommended.


Incubate the plate for 30 minutes at room temperature (23 ± 3°C).

- c. Wash the wells 4 times as in step a.
- d. Rapidly (preferably using an 8-channel pipette) dispense the conjugate (14 mL, ready-to-use, red); 100 µL per well. Incubate the plate as in step b.
- e. Repeat wash step c.
- f. Rapidly (preferably using an 8-channel pipette) dispense the substrate solution (14 mL, ready-to-use, colourless, black vial); 100 µL per well. Incubate the plate as in step b. As the substrate is photosensitive, avoid intense light exposure (e.g. direct sunlight) during incubation.
- g. Rapidly (preferably using an 8-channel pipette) dispense the stop solution (14 mL, ready-to-use, colourless. Caution: corrosive!); 100 µL per well. Use the same sequence as for the substrate. The colour changes from blue to yellow. Agitate the plate, preferably on an orbital shaker, for about 10 seconds.
- h. Immediately read the absorbance in the microwell plate photometer at 450 nm.

Refrigerate the remainder of the reagents (2 - 8°C) if they are to be used again.

9. Evaluation and quality control

Quantitative evaluation: the data obtained are quantitatively evaluated with the standard curve, as shown below. However, the depicted curve can only serve as a model. It can not substitute the measurement of the calibrators, together with the controls and actual samples. The curve has been constructed with a conventional ELISA evaluation program, using a 4-parameter function. The Spline approximation is also appropriate.

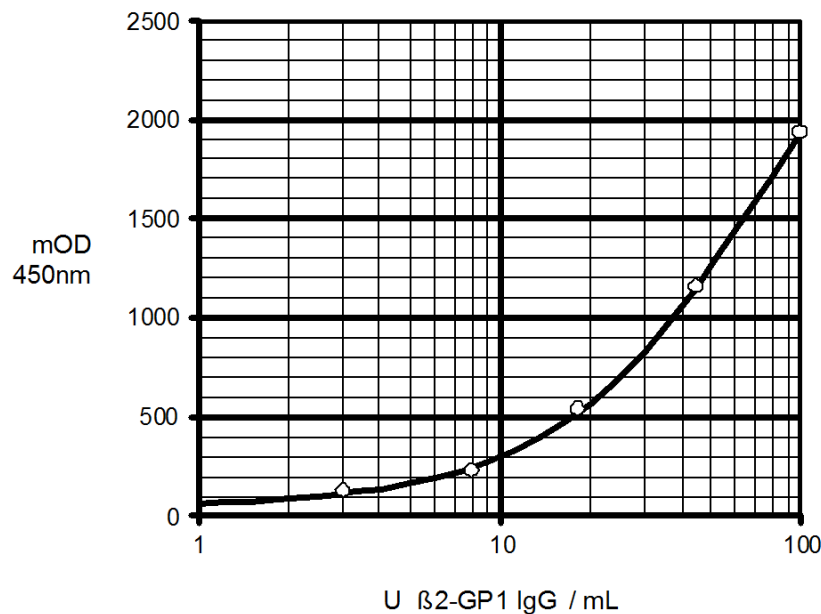

If no computer-supported evaluation is possible, the standard curve may be drawn by hand. It allows transformation of the absorbance value of a sample into its concentration, i.e. into U β2-GP1 IgG per mL sample.

Qualitative evaluation: the test may also be evaluated in a qualitative manner. This requires measurement of the positive control only. Nevertheless, measurement and examination of the negative control is recommended (see below: quality control).

In qualitative test evaluation, the absorbance of the samples is compared with the borderline absorbance (= cut-off). It is determined according to the following formula:

$$\text{absorbance}_{\text{borderline}} = \text{absorbance}_{\text{positive control}} \times \text{factor}$$

The factor depends on the kit lot and is quoted in the lot-specific certificate of analysis which is included with each test kit. Example:

$$\text{absorbance}_{\text{positive control}} = 1250 \text{ mOD}$$

$$\text{factor} = 0,35$$

$$\text{absorbance}_{\text{borderline}} = 1250 \text{ mOD} \times 0,35 = 438 \text{ mOD}$$

In order to gain an impression of how positive a particular sample is for β2-GP1 IgG, one may calculate the ratio, according to the formula:

$$\text{ratio} = \text{absorbance}_{\text{sample}} / \text{absorbance}_{\text{borderline}}$$

Example:

$$\text{absorbance}_{\text{borderline}} = 438 \text{ mOD}$$

$$\text{absorbance}_{\text{sample}} = 1480 \text{ mOD}$$

$$\text{ratio} = 1480 \text{ mOD} / 438 \text{ mOD} = 3,4$$

Quality control: the positive and negative control check the assay performance. Their authorised values and acceptable ranges, respectively, are quoted in the lot-specific certificate of analysis. Values of the controls must fall within the indicated ranges; otherwise, the results of the assay are invalidated.

10. Interpretation of results / limitations of the procedure

Based on the measurement of a blood donor and a positive collective of sera (see below), we suggest for the assessment of patient sera:

	quantitative evaluation U β 2-GP1 IgG / mL sample	qualitative evaluation ratio
normal (negative) range	< 10,0	< 0,84
cut-off	12,0	1,00
equivocal range	10,0 - 14,4	0,84 - 1,19
positive range	> 14,4	> 1,19

These specifications are given as an indication only; in order to check their accuracy, each analysis should include parallel samples of normal sera.

A negative test result indicates that the patient does not have an elevated level of IgG antibodies to β 2-GP1. If characteristic clinical signs of APS are nevertheless observed, IgA/IgM antibodies directed at β 2-GP1 and/or antibodies directed at CL should be determined.

A positive result should be considered as an indication for APS, as outlined in the beginning. However, it needs to be positive on at least two occasions, separated by 12 weeks, to be considered diagnostic for APS (1).

Specimens exhibiting results within the borderline range quoted above should be considered as equivocal and reported as such. It is recommended that a second sample be collected two weeks later and run in parallel with the first sample to document a possible change of antibody titer.

As with any serological test, the results should be interpreted in the light of the patient's symptoms and other diagnostic criteria.

11. Performance characteristics

11.1. Standardisation

The test is standardised with a purified serum preparation containing IgG antibodies specifically directed at β 2-GP1. This preparation is calibrated against the "DeBari" standard serum (11). The degree of sample reactivity is measured in relative ("DeBari")-units (U β 2-GP1 IgG / mL).

11.2. Analytical specificity

The test allows the specific determination of human IgG antibodies directed against β 2-GP1.

11.3. Detection limit (analytical sensitivity)



The detection limit is defined as that concentration of analyte that corresponds to the mean absorbance of sample buffer plus 3-fold standard deviation (s). It was determined as < 0,5 U β 2-GP1 IgG per mL sample (n = 24).

Recommended measuring range: 2 - 100 U β 2-GP1 IgG per mL sample

11.4. Homogeneity of the solid phase


Measurement of the solid phase homogeneity is a regular QC part of each production lot. This is determined by 288-fold measurement of an IgG-positive but non-saturating sample on 3 selected plates. Acceptance criterion: mOD-coefficient of variation (cv) over the plates < 8%. The figure below shows a representative excerpt (solid phase lot no. 0104S) of such an analysis.

plate row	1	n/2	n	1	n/2	n	1	n/2	n	1	n/2	n	mean	cv %
	1	1	1	2	2	2	3	3	3	4	4	4		
line a	1496	1505	1585	1455	1516	1519	1546	1505	1526	1413	1510	1572	1512	3,1
line b	1498	1516	1581	1465	1526	1550	1444	1516	1559	1425	1512	1628	1518	3,8
line c	1520	1517	1544	1473	1520	1533	1440	1518	1545	1434	1510	1617	1514	3,2
line d	1481	1479	1541	1449	1512	1549	1463	1534	1554	1445	1542	1580	1511	3,0
line e	1508	1547	1586	1497	1507	1545	1476	1537	1604	1441	1542	1606	1533	3,3
line f	1503	1493	1578	1480	1476	1547	1461	1528	1599	1473	1545	1622	1525	3,5
line g	1489	1501	1577	1467	1513	1558	1495	1526	1577	1504	1574	1609	1533	2,9
line h	1447	1440	1519	1451	1433	1467	1464	1487	1499	1450	1508	1560	1477	2,6
mean	1493	1500	1564	1467	1500	1534	1474	1519	1558	1448	1530	1599	1515	
cv %	1,5	2,1	1,6	1,1	2,1	1,9	2,3	1,1	2,3	2,0	1,6	1,6		3,3

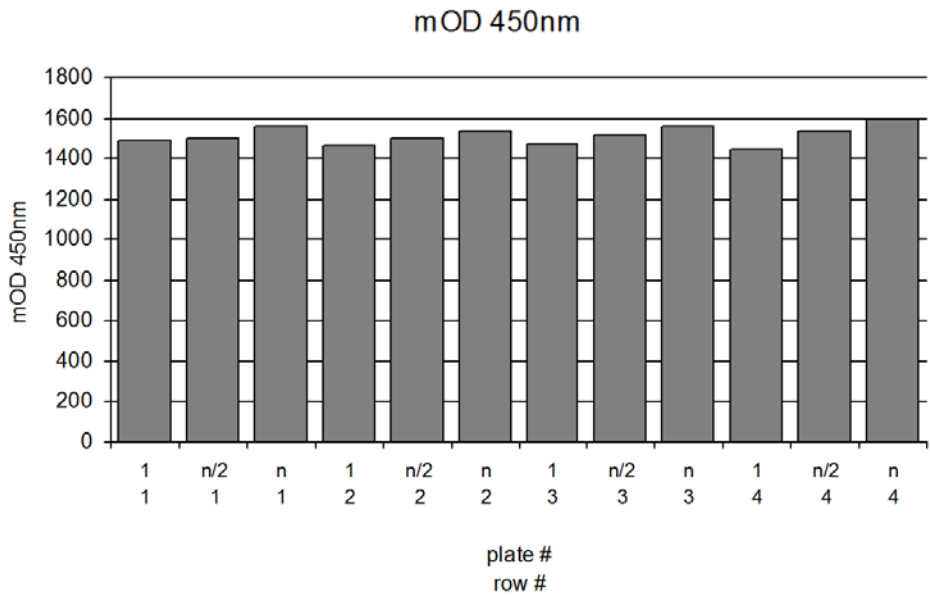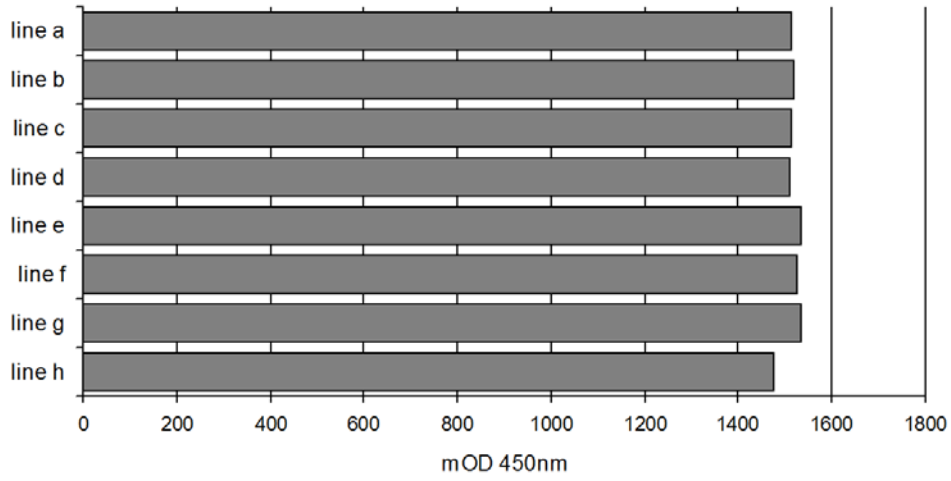

11.5. Linearity

In order to assess the dose-response relationship of the test, positive sera were measured in serial 2-fold dilution. Acceptance criterion: linear regression of 4 successive dilutions must yield a correlation factor > 0,98. A typical result is depicted below.

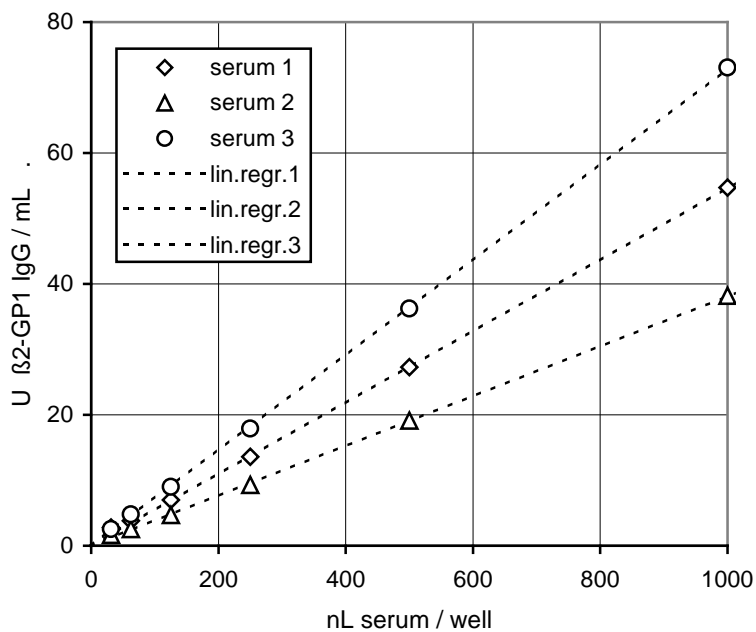

11.6. Precision

For the assessment of the test precision, the variability of results under the following conditions was determined: a. within 1 assay and between 3 assays, b. between 3 operators and c. between 2 kit lots.

a. Intra- and inter-assay variability (n = 24 and 72, respectively)

sample	mean U/mL	variability (cv, %)	
		intra-assay	inter-assay
1	12	4,8	5,2
2	20	4,3	5,0
3	43	6,4	7,4

b. Operator to operator variability (n = 12)

sample	mean U/mL	variability (cv, %)
1	14	3,9
2	25	3,3
3	43	2,3

c. Variability between 2 kit lots (n = 6)

sample	mean U/mL	variability (cv, %)
1	15	10,0
2	25	8,5
3	52	10,4


11.7. Frequency distribution of β 2-GP1 IgG

This was analysed in a sera collective of blood donors, equally distributed by sex and age, and a collective of positive sera according to a CE-compliant reference ELISA. The following distribution of the analyte was observed:


blood donor sera	positive sera
n: 160	n: 22
mean: 3,7 U/mL	mean: 130 U/mL
mean + s: 8,6 U/mL	mean - s: < 0 U/mL
mean + 2s: 13,5 U/mL	mean - 2s: < 0 U/mL
median: 2,7 U/mL	median: 88 U/mL
95 th percentile: 6,7 U/mL	5 th percentile: 18 U/mL

ROC-analysis of these data was used to determine the cut-off as 12,0 U β 2-GP1 IgG / mL (12). The data presented here suggest a diagnostic specificity and sensitivity of the ELISA of about 97 and nearly 100 %, respectively. These values apply for the measured sera only; other collectives may yield different results. In view of the low number of positive sera, particular caution is required when interpreting test sensitivity.

blood donor sera

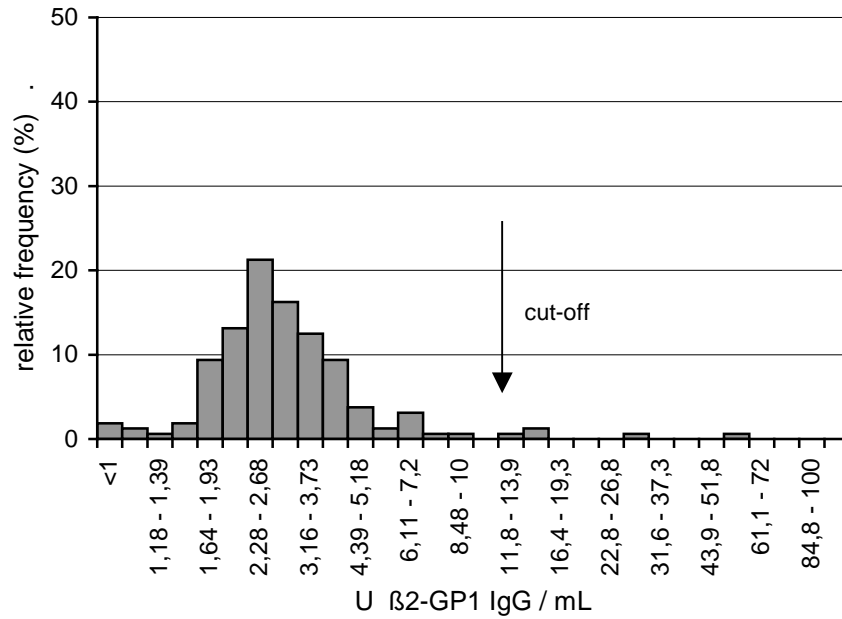

positive sera

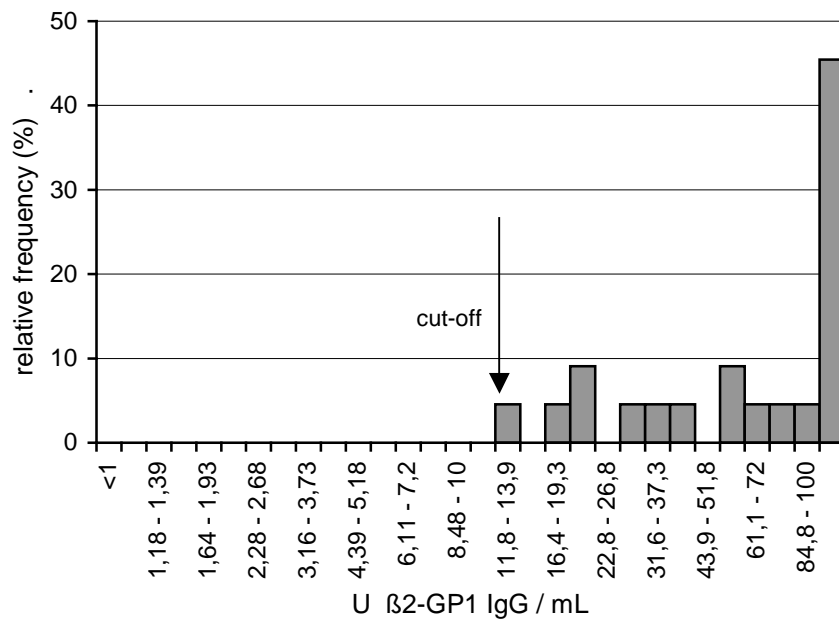

12. Warranty

IBL International GmbH guarantees that the product delivered has been thoroughly tested to ensure that its properties specified herein are fulfilled. No further warranties are given.

The performance data presented here were obtained using the procedure indicated. Any modification in the procedure may affect the results in which case IBL disclaims all warranties whether expressed, implied or statutory. Moreover, IBL accepts no liability for any damage, whether direct, indirect or consequential, which results from inappropriate use or storage of the product.

13. References

1. Ortel, T. L.: Antiphospholipid Syndrome Laboratory Testing and Diagnostic Strategies. *Am J Hematol.* 87 (2012), 75 - 81
2. Gromnica-Ihle, E., and Schössler, W.: Antiphospholipid Syndrome. *Int Arch Allergy Immunol* 123 (2000), 67 - 76
3. Harris, E. N., et al.: Anticardiolipin antibodies: Detection by radioimmunoassay and association with thrombosis in systemic lupus erythematosus. *Lancet* Nov 26 (1983), 1211 - 1214
4. Petri, M.: Epidemiology of the Antiphospholipid Antibody Syndrome. *J Autoimm* 15 (2000), 145 - 151
5. Galli, M., et al.: Anticardiolipin antibodies (ACA) directed not to cardiolipin but to a plasma cofactor. *Lancet* 335 (1990), 1544 - 1547
6. Matsuura, E., et al.: Anticardiolipin antibodies recognise β 2-Glycoprotein 1 structure altered by interacting with an oxygen modified solid phase surface. *J Exp Med* 179 (1994), 457 - 462
7. Lopez, L. R., et al.: Anti- β 2-glycoprotein I and antiphosphatidylserine antibodies are predictors of arterial thrombosis in patients with antiphospholipid syndrome. *Am J Clin Pathol* 121 (2004), 142 - 149
8. Kelchtermans, H., et al.: IgG/IgM antiphospholipid antibodies present in the classification criteria for the antiphospholipid syndrome: a critical review of their association with thrombosis. *Journal of Thrombosis and Haemostasis* 14 (2016), 1530 - 1548
9. Shoenfeld, Y., et al.: Induction and treatment of the antiphospholipid syndrome - lessons from animal models. *Eur J Clin Invest* 31 (2001), 736 - 740
10. Pierangeli, S. S., et al.: Complement activation: a novel pathogenic mechanism in the antiphospholipid syndrome. *Ann NY Acad Sci* 1051 (2005), 413 - 420
11. Erickson, E. N., et al.: Reference calibrators for IgG antibodies to β 2-GP1: Preparation, properties, and availability to investigators. *Clin. Chem.* 42 (1996), 1116-1117
12. Sommer, R., and Eitelberger, F.: Wertigkeit der Gliadin-Antikörper im Serum zur Diagnose der Zöliakie. *Wien Klin Wochenschr* 104/4 (1992), 86 - 92

14. Summary flow chart

- a. Dilute the samples 1/100 in sample buffer (100 mL, ready-to-use, orange) and mix.
- b. Dilute the wash buffer 10x-concentrate (100 mL, blue) with water and mix.
- c. Wash the wells once with 350 μ L wash buffer each. Dispense 100 μ L of the calibrators (2,0 mL each, ready-to-use, gradually blue) and controls (2,0 mL each, ready-to-use, green and red) and of the diluted samples into the wells of the solid phase. Duplicate measurements are recommended. Incubate for 30 minutes at room temperature ($23 \pm 3^\circ\text{C}$).
- d. Wash the wells 4 times with 350 μ L wash buffer each.
- e. Dispense 100 μ L of the conjugate (14 mL, ready-to-use, red) into the wells. Incubate as in step c.
- f. Repeat washing step d.
- g. Dispense 100 μ L of the substrate solution (14 mL, ready-to-use, black vial) per well. Incubate as in step c. Then, add 100 μ L stop solution (14 mL, ready-to-use, colourless) per well and agitate the plate briefly.
- h. Immediately measure the absorbance at 450 nm.
- i. Quantitative evaluation: determine the standard curve and, using this curve, transform the absorbance of the samples into their respective antibody concentration (U/mL).
- j. Qualitative evaluation: determine the borderline absorbance by multiplying the absorbance of the positive control with the factor shown in the certificate of analysis. Then, calculate the ratio of the samples by dividing their absorbance by the borderline absorbance.

Symbols / Symbole / Symbôles / Símbolos / Símbolos / Σύμβολα

	Cat.-No.: / Kat.-Nr.: / No.- Cat.: / Cat.-No.: / N.º Cat.: / N.-Cat.: / Αριθμός-Κατ.:
	Lot-No.: / Chargen-Bez.: / No. Lot: / Lot-No.: / Lote N.º: / Lotto n.: / Αριθμός -Παραγωγή:
	Use by: / Verwendbar bis: / Utiliser à: / Usado por: / Usar até: / Da utilizzare entro: / Χρησιμοποιείται από:
	No. of Tests: / Kitgröße: / Nb. de Tests: / No. de Determ.: / N.º de Testes: / Quantità dei tests: / Αριθμός εξετάσεων:
	Concentrate / Konzentrat / Concentré / Concentrar / Concentrado / Concentrato / Συμπύκνωμα
	Lyophilized / Lyophilisat / Lyophilisé / Liofilizado / Liofilizado / Liofilizzato / Λυοφιλιασμένο
	In Vitro Diagnostic Medical Device. / In-vitro-Diagnostikum. / Appareil Médical pour Diagnostics In Vitro. / Dispositivo Médico para Diagnóstico In Vitro. / Equipamento Médico de Diagnóstico In Vitro. / Dispositivo Medico Diagnostico In vitro. / Ιατρική συσκευή για In-Vitro Διάγνωση.
	Evaluation kit. / Nur für Leistungsbewertungszwecke. / Kit pour évaluation. / Juego de Reactivos para Evaluació. / Kit de avaliação. / Kit di valutazione. / Κιτ Αξιολόγησης.
	Read instructions before use. / Arbeitsanleitung lesen. / Lire la fiche technique avant emploi. / Lea las instrucciones antes de usar. / Ler as instruções antes de usar. / Leggere le istruzioni prima dell'uso. / Διαβάστε τις οδηγίες πριν την χρήση.
	Keep away from heat or direct sun light. / Vor Hitze und direkter Sonneneinstrahlung schützen. / Garder à l'abri de la chaleur et de toute exposition lumineuse. / Manténgase alejado del calor o la luz solar directa. / Manter longe do calor ou luz solar directa. / Non esporre ai raggi solari. / Να φυλάσσεται μακριά από θερμότητα και άμεση επαφή με το φως του ηλίου.
	Store at: / Lagern bei: / Stocker à: / Almacene a: / Armazemar a: / Conservare a: / Αποθήκευση στους:
	Manufacturer: / Hersteller: / Fabricant: / Productor: / Fabricante: / Fabbicante: / Παραγωγός:
	Caution! / Vorsicht! / Attention! / ¡Precaución! / Cuidado! / Attenzione! / Προσοχή!
<p>Symbols of the kit components see MATERIALS SUPPLIED. Die Symbole der Komponenten sind im Kapitel KOMPONENTEN DES KITS beschrieben. Voir MATERIEL FOURNI pour les symbôles des composants du kit. Símbolos de los componentes del juego de reactivos, vea MATERIALES SUMINISTRADOS. Para símbolos dos componentes do kit ver MATERIAIS FORNECIDOS. Per i simboli dei componenti del kit si veda COMPONENTI DEL KIT. Για τα σύμβολα των συστατικών του κιτ συμβουλευτείτε το ΠΑΡΕΧΟΜΕΝΑ ΥΛΙΚΑ.</p>	

COMPLAINTS: Complaints may be submitted initially written or vocal. Subsequently they need to be filed including the test performance and results in writing in case of analytical reasons.

WARRANTY: The product is warranted to be free from material defects within the specific shelf life and to comply with product specifications delivered with the product. The product must be used according to the Intended use, all instructions given in the instructions for use and within the product specific shelf life. Any modification of the test procedure or exchange or mixing of components of different lots could negatively affect the results. These cases invalidate any claim for replacement.

LIMITATION OF LIABILITY: IN ALL CIRCUMSTANCES THE EXTENT OF MANUFACTURER'S LIABILITY IS LIMITED TO THE PURCHASE PRICE OF THE KIT(S) IN QUESTION. IN NO EVENT SHALL MANUFACTURER BE LIABLE FOR ANY INCIDENTAL OR CONSEQUENTIAL DAMAGES, INCLUDING DAMAGES FOR LOST PROFITS, LOST SALES, INJURY TO PERSON OR PROPERTY OR ANY OTHER INCIDENTAL OR CONSEQUENTIAL LOSS.



IBL International GmbH

Flughafenstrasse 52a
D-22335 Hamburg, Germany

Phone: +49 (0)40-53 28 91-0
Fax: +49 (0)40-53 28 91-11

IBL@tecan.com
www.tecan.com/ibl

Always there for you

