




Instructions for use

ANA Screen 8 ELISA

Enzyme immunoassay for the qualitative screening of IgG antibodies against dsDNA, RNP, Sm, SS-A/Ro, SS-B/La, Scl-70, CENP-B and Jo-1 in human serum or plasma (EDTA, citrate).

REF RE75421

 12x8

  2°C  8°C

EU: **IVD**  



IBL International GmbH
Flughafenstrasse 52a
D-22335 Hamburg, Germany

Always there for you



1. Introduction and background

Circulating autoantibodies against various intracellular antigens (antinuclear antibodies, ANA) are characteristic for systemic, autoimmune-mediated rheumatic diseases of the connective tissue (1, 2, 3, 4). These comprise Systemic Lupus Erythematosus (SLE), Mixed Connective Tissue Disease (MCTD), Sjögren's Syndrome (SS) A and B, Progressive Systemic Sclerosis (PSS, Scleroderma)/CREST Syndrome and Polymyositis (PM).

The diagnosis of the above disorders is often difficult, due to overlapping symptoms, and therefore usually supported by measuring their associated autoantibodies. 8 antigens specifically recognised by these antibodies are immobilised on the solid phase of the present enzyme-linked immuno sorbent assay (ELISA):

antigen	source	disease	approximate autoantibody prevalence (5)
dsDNAplasmid RNP (proteins A, C, 68kDa)	SLE recombinant	60 - 90 %	
		MCTD	95 %
		SLE	30 - 40 %
		PM	14 %
Sm (proteins B, B', D)	bovine thymus	SS	4 %
		SLE	12 - 39 %
		MCTD	7 %
		SS	60 - 100 %
SS-A/Ro (60kDa-protein)	bovine thymus	SLE	45 - 50 %
		MCTD	15 - 30 %
		PSS	5 - 7 %
		PM	5 - 7 %
		SS	30 - 90 %
SS-B/La	recombinant	SLE	15 - 30 %
		MCTD	5 - 15 %
		PSS	20 - 76 %
Scl-70 (DNA-topoisomerase 1)	recombinant	CREST	40 - 80 %
CENP-B (centromere protein B)	recombinant	PM	20 - 40 %
Jo-1 (Histidyl-tRNA-synthetase)	recombinant		

The test is designed for the qualitative, summary determination of the respective autoantibodies (IgG) in human serum or plasma (cf. section 7), without the ability to discriminate between them. It is intended as initial screen test for an overall diagnosis of the above disorders. The test is fast (incubation time 30 / 30 / 30 minutes) and flexible (divisible solid phase, ready-to-use reagents). A negative and a positive control check the assay performance. The positive control also serves as calibrator for assay evaluation.

2. Warnings and precautions

The test kit is intended for in vitro diagnostic use only; not for internal or external use in humans or animals. It must be executed by trained personnel staff.

Do not use reagents beyond their expiration dates. Adherence to the protocol is strongly recommended.

The sample buffer and controls contain Na-azide as antimicrobial agent. The wash buffer contains bromonitrodioxane and the conjugate methylisothiazolone / bromonitrodioxane as preservative. The substrate contains 3, 3', 5, 5'-tetramethylbenzidine (TMB) and hydrogen peroxide (H₂O₂). The stop solution, 0,2 M sulfuric acid (H₂SO₄), is acidic and corrosive.

The above mentioned reagents may be toxic if ingested. Follow routine precautions for handling hazardous chemicals. Avoid all body contact, wear gloves and eye protection. If one of the reagents comes into contact with skin or mucous membrane, wash thoroughly with water. Never pipette by mouth. Dispose in a manner complying with local/national regulations.

Na-Azide may react with lead and copper plumbing to form explosive metal azides. On disposal, flush with a large amount of water to prevent azide build-up.

The controls contain components of human origin. They were tested for human immunodeficiency virus (HIV)-Ag, hepatitis B surface (HBs)-Ag and antibodies against HIV 1/2 and hepatitis C virus (HCV) and showed negative results; either in an FDA-approved or a CE-compliant test, according to European Directive 98/79/EC.

However, no test can guarantee that material of human origin is not actually infectious. The preparations should therefore be treated as potentially infectious and disposed of accordingly, as should the samples (and residues thereof); according to CDC (Center of Disease Control, Atlanta, USA) or other local / national guidelines on laboratory safety and decontamination.

3. Principle of the test

The wells of the solid phase are coated with a balanced mixture of the autoantigens quoted above. On this surface, the following immunological reactions take place:

1st reaction: Antigen-specific antibodies present in the sample bind to the respective immobilised antigen, forming the antigen-antibody complex. Then, non-bound sample components are washed away from the solid phase.

2nd reaction: A second antibody, directed at human IgG antibodies and conjugated with horse-radish peroxidase (HRP), is added. This conjugate binds to the complex. Then, excess conjugate is washed away from the solid phase.

3rd reaction: The enzyme-labelled complex converts a colourless substrate into a blue product. The degree of colour development reflects the total concentration of all antigen-specific IgG autoantibodies in the sample.

4. Contents of the kit

- a. **MTP** 1 **Microtiter Plate**, coated with a mixture of the above antigens, hermetically packed in a foil laminate pouch together with a desiccant bag. The plate consists of 12 strips, each of which can be broken into 8 individual wells.
- b. **SAMPLEDIL** **Sample Diluent**, 100 mL, ready-to-use, orange coloured. Contains Tris-buffered saline (TBS), bovine serum albumin (BSA), Tween and Na-azide.
- c. **WASHBUF** **CONC** **Wash buffer**, 100 mL, 10x-concentrate, blue coloured. Contains TBS, Tween and bromonitrodioxane.
- d. **CONTROL +** **CONTROL -** **Negative and Positive Control**, 3,0 mL each, ready-to-use, green and red coloured, respectively. Contain TBS, BSA, Tween and Na-azide.
- e. **ENZCONJ IgG** **Enzyme Conjugate**, 14 mL, ready-to-use, red coloured. Buffered solution containing stabilising protein, methylisothiazolone and bromonitrodioxane.
- f. **TMB SUBS** **TMB Substrate Solution**, 14 mL, ready-to-use, colourless. Contains a buffered solution of TMB and H₂O₂. Contained in a vial impermeable to light.
- g. **STOP** **TMB Stop Solution** (0,2 M H₂SO₄), 14 mL, colourless, ready-to-use. Caution: sulfuric acid is corrosive.
- h. Directions for use
- i. Lot-specific certificate of analysis

5. Materials required but not supplied

- a. Deionised or distilled water
- b. Graduated cylinder, 1000 mL
- c. Tubes for sample dilution (transfer tubes in the microwell plate format recommended)
- d. Pipettes for 10, 100 and 1000 µL (1- and 8-channel pipettes recommended)
- e. Microwell plate washer (optional)
- f. Microwell plate photometer fitted with a 450 nm filter
- g. ELISA evaluation program (recommended)

6. Storage of the kit

Store kit at 2 - 8°C. It is stable up to the expiry date stated on the label of the box. Do not use kit beyond its expiry date.

7. Reagent and sample preparation / specimen requirements

Do not exchange or pool corresponding components from different kits, due to possibly different shipping or storage conditions. If the kit is to be used for several tests, only the currently needed amount of reagents should be withdrawn. It is **crucially important** that no cross-contamination between the reagents occurs. Use only clean pipettes and do **not pour back** residues into the original flasks.

- a. The solid phase must reach room temperature before opening the pouch. Remove the supernumerary microwells from the frame and immediately put them back into the pouch, together with the desiccant bag. Reseal the pouch hermetically and keep it refrigerated for future use.
- b. Dilute the wash buffer 10x-concentrate (100 mL, blue) with 900 mL deionised water. Mix thoroughly. The diluted buffer is stable for several weeks if stored refrigerated (2 - 8°C).
- c. Preparation of the samples: handle patient specimens as potentially infectious agents. Besides serum, EDTA- or citrate-treated plasma are suitable sample material as well; heparin-treated plasma however is not.

Specimen requirements: highly lipemic, haemolysed or microbially contaminated samples may cause erroneous results and should be avoided.

Prepare samples using normal laboratory techniques. Turbid samples must first be clarified (centrifuged). The clarified or clear samples are mixed and then diluted 1/100, e.g. 10 µL serum or plasma + 990 µL sample buffer. Also mix the dilution.

For rapid dispensing during the assay procedure, preparation of the controls and samples in microwell transfer tubes is recommended. This allows the operation of an 8-channel pipette during the assay procedure.

If samples are not assayed immediately, they should be stored at 2 - 8°C and assayed within 3 days. For longer storage, -20°C or lower temperatures are recommended. Repeated freezing and thawing of samples should be avoided. Thawed samples must be mixed prior to diluting.

8. Assay procedure

8.1. Manual operation

Before starting the assay, all components of the kit must have reached room temperature ($23 \pm 3^{\circ}\text{C}$).

To achieve best results, i.e. the maximum ratio between specific and background signal, **careful washing** is essential (steps a, c and e). It is **crucially important to remove the wash solution completely**. For that purpose, tap the plate firmly on several layers of absorbent tissue. Automated washers must be verified according to results obtained by manual washing.

a. Immediately prior to use, wash the solid phase once: fill wells with 350 μL wash buffer each, let soak for about 10 seconds in the wells and remove.

b. Dispense the controls (3,0 mL each, ready-to-use, green and red) and the diluted samples rapidly into the microwells; 100 μL per well. Duplicate measurements are recommended.

Incubate the plate for 30 minutes at room temperature ($23 \pm 3^{\circ}\text{C}$).

c. Wash the wells 4 times as in step a.

d. Rapidly (preferably using an 8-channel pipette) dispense the conjugate (14 mL, ready-to-use, red); 100 μL per well. Incubate the plate as in step b.

e. Repeat wash step c.

f. Rapidly (preferably using an 8-channel pipette) dispense the substrate solution (14 mL, ready-to-use, colourless, black vial); 100 μL per well. Incubate the plate as in step b. As the substrate is photosensitive, avoid intense light exposure (e.g. direct sunlight) during incubation.

g. Rapidly (preferably using an 8-channel pipette) dispense the stop solution (14 mL, ready-to-use, colourless. Caution: corrosive!); 100 μL per well. Use the same sequence as for the substrate. The colour changes from blue to yellow. Agitate the plate, preferably on an orbital shaker, for about 10 seconds.

h. Immediately read the absorbance in the microwell plate photometer at 450 nm.

Refrigerate the remainder of the reagents ($2 - 8^{\circ}\text{C}$) if they are to be used again.

9. Evaluation and quality control

The assay is evaluated in a qualitative manner: the absorbance of the samples is compared to the borderline absorbance (= cut-off absorbance). The cut-off absorbance is determined by means of the positive control which at the same time functions as calibrator; according to the formula:

$$\text{absorbance}_{\text{borderline}} = \text{absorbance}_{\text{positive control}} \times \text{factor}$$

The factor depends on the kit lot and is quoted in the lot-specific certificate of analysis (included with each test kit). Example:

$$\begin{aligned} \text{absorbance}_{\text{positive control}} &= 1250 \text{ mOD} \\ \text{factor} &= 0,35 \\ \text{absorbance}_{\text{borderline}} &= 1250 \text{ mOD} \times 0,35 = 438 \text{ mOD} \end{aligned}$$

In order to gain an impression of the degree of a sample's reactivity, the ratio between sample and borderline absorbance is calculated:

$$\text{ratio} = \text{absorbance}_{\text{sample}} / \text{absorbance}_{\text{borderline}}$$

Example:

$$\begin{aligned} \text{absorbance}_{\text{borderline}} &= 438 \text{ mOD} \\ \text{absorbance}_{\text{sample}} &= 1480 \text{ mOD} \\ \text{ratio} &= 1480 \text{ mOD} / 438 \text{ mOD} = 3,4 \end{aligned}$$

Quality control: the positive control (calibrator) and negative control check the assay performance. Their acceptable ranges are quoted in the lot-specific certificate of analysis. Values of the controls must fall within the indicated ranges; otherwise, the results of the assay are invalidated.

10. Interpretation of results / limitations of the procedure

Based on the measurement of a blood donor and a positive collective of sera (see below), we suggest for the assessment of patient sera:

	ratio
normal (negative) range	< 0,82
cut-off	1,00
equivocal range	0,82 - 1,20
positive range	> 1,20

These specifications are given as an indication only; in order to check their accuracy, each analysis should include parallel samples of normal sera.

A negative test result indicates that the patient probably does not have an elevated level of IgG antibodies to the antigens listed in the beginning. Therefore, presence of a systemic rheumatic disease is rather unlikely but can nevertheless not be excluded.

A positive result should be considered as an indication for one of the above listed diseases. As follow-up diagnosis, the specificity of the causative autoantibody and hence the identity of the autoimmune disorder should be determined. This can be achieved by means of a differentiating profile ELISA.

Specimens exhibiting results within the borderline range quoted above should be considered as equivocal and reported as such. It is recommended that a second sample be collected two weeks later and run in parallel with the first sample to document a possible change of antibody titer.

As with any serological test, the results should be interpreted in the light of the patient's symptoms and other diagnostic criteria.

11. Performance characteristics

11.1. Standardisation

The test is standardised with a purified serum preparation containing IgG antibodies directed at each of the immobilised autoantigens. It constitutes the stock material for both controls of the test. The proportion of the antibodies is adjusted in such a manner that each one contributes approximately the same fraction to the overall signal.

The stock preparation is calibrated against a set of monospecifically positive sera solely reserved for this purpose. The degree of sample reactivity is expressed as summary ratio, as outlined above.

11.2. Analytical specificity

The test permits the specific determination of human IgG antibodies, directed at the autoantigens quoted in article 1. It has been validated (among other criteria) using human reference sera from the Center of Disease Control (CDC; Atlanta, USA) which are commercially available. The following results (ratio values) are typical:

Serum	1	2	3	4	5	6	7	8	9	10
CDC- result	ds- DNA	SS-B /La	--	U1- RNP	Sm	--	SS-A /Ro	--	Scl- 70	Jo- 1
Immun- fluoresc. ratio	homo- gen	speck- led	speck- led	--	--	nuc- leolar	--	centro- mere	--	--
	5,0	11	9,4	3,8	9,2	1,2	6,6	5,9	6,6	9,4

Remark: The corresponding ANA Profile 8 IgG ELISA which differentiates between the antigens revealed that serum # 6 shows ratio values ≤ 1 towards all single antigens.

11.3. Detection limit (analytical sensitivity)



The detection limit is defined as that concentration of analyte that corresponds to the mean absorbance of sample buffer plus 3-fold standard deviation (s). It was determined as $< 0,3$ (ratio; $n = 24$).

Recommended measuring range: $0,4 < \text{ratio} < 6$

11.4. Homogeneity of the solid phase


Measurement of the solid phase homogeneity is a regular QC part of each production lot. This is determined by 288-fold measurement of a positive but non-saturating sample on 3 selected plates. Acceptance criterion: mOD-coefficient of variation (cv) over the plates $< 8\%$. The figure below shows a representative excerpt (solid phase lot no. 0511R) of such an analysis.

plate row	1 1	n/2 1	n 1	1 2	n/2 2	n 2	1 3	n/2 3	n 3	1 4	n/2 4	n 4	mean	cv %
line a	771	798	776	759	760	762	776	794	765	765	774	761	772	1,7
line b	800	816	785	812	817	802	793	822	789	805	804	809	804	1,4
line c	762	801	773	787	791	779	785	818	787	790	783	793	787	1,8
line d	755	798	779	785	801	778	780	800	800	788	787	804	788	1,8
line e	789	829	820	789	813	802	794	826	803	792	818	818	808	1,8
line f	793	823	801	785	806	799	795	827	810	800	837	834	809	2,1
line g	798	829	828	807	822	809	806	832	820	800	838	850	820	2,0
line h	767	801	805	773	795	789	783	795	784	780	806	834	793	2,3
mean	779	812	796	787	801	790	789	814	794	790	806	813	798	
cv %	2,2	1,7	2,6	2,2	2,4	2,0	1,3	1,9	2,2	1,6	3,0	3,4		2,6

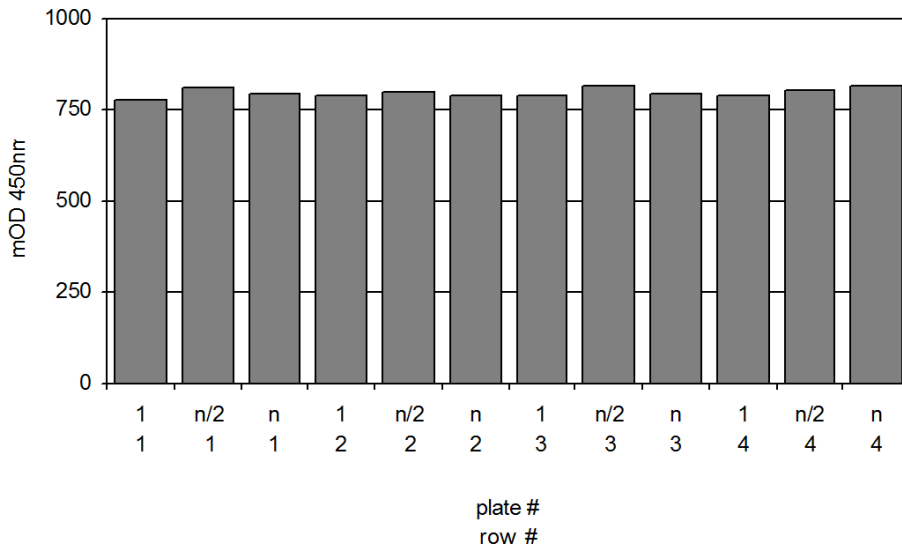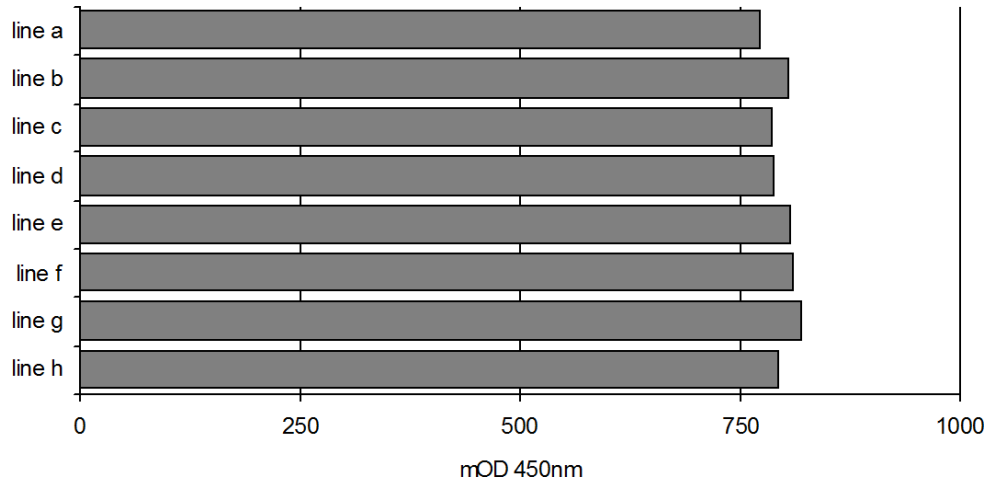

11.5. Dose-response relationship

In order to assess this feature of the ELISA, several pools of individual sera with heterogeneous reactivity were measured in serial 2-fold dilution. A typical result is depicted below. An approximately linear relationship between sample concentration and resulting ratio is restricted to ratio values < 2. This is due to the qualitative evaluation manner (cf. article 9) and contrasts ELISAs which are evaluated quantitatively by means of a standard curve.

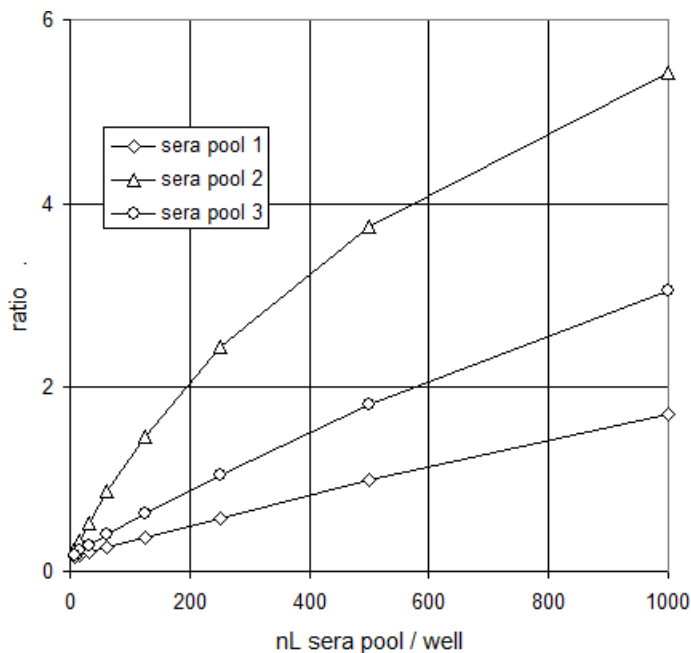

11.6. Precision

For the assessment of the test precision, the variability of results under the following conditions was determined: a. within 1 assay and between 3 assays, b. between 3 operators and c. between 2 kit lots.

a. Intra- and inter-assay variability (n = 24 and 72, respectively)

sample	ratio	variability (cv, %)	
		intra-assay	inter-assay
1	1,4	1,9	2,1
2	2,4	2,0	2,1
3	4,0	1,4	1,7

b. Operator to operator variability (n = 12)

sample	ratio	variability (cv, %)
1	1,4	2,5
2	2,4	1,8
3	4,0	2,9

c. Variability between 2 kit lots (n = 6)

sample	ratio	variability (cv, %)
1	1,3	4,9
2	2,3	5,3
3	3,8	3,8

11.7. Frequency distribution of ANAs (IgG)


This was analysed in a sera collective of blood donors, equally distributed by sex and age, and a collective of sera which had been found positive by independent methods (e.g. monospecific, CE-compliant reference ELISAs, immune fluorescence assays (IFA)) for at least one parameter or were clinically defined.

The following summary distribution of the analytes was observed (s = standard deviation):


blood donor sera		positive sera	
n:	160	n:	83
mean:	ratio = 0,64	mean:	ratio = 7,5
mean + s:	ratio = 1,08	mean - s:	ratio = 4,9
mean + 2s:	ratio = 1,53	mean - 2s:	ratio = 2,4
median:	ratio = 0,54	median:	ratio = 8,2
95 th percentile:	ratio = 1,14	5 th percentile:	ratio = 2,5

ROC-analysis of these data was used to determine the cut-off of the ANA Screen 8 IgG ELISA according to (6). The data presented here suggest a diagnostic specificity and sensitivity of the ELISA of about 91 and nearly 100 %, respectively. These values apply for the measured sera only; other collectives may yield different results.

blood donor sera

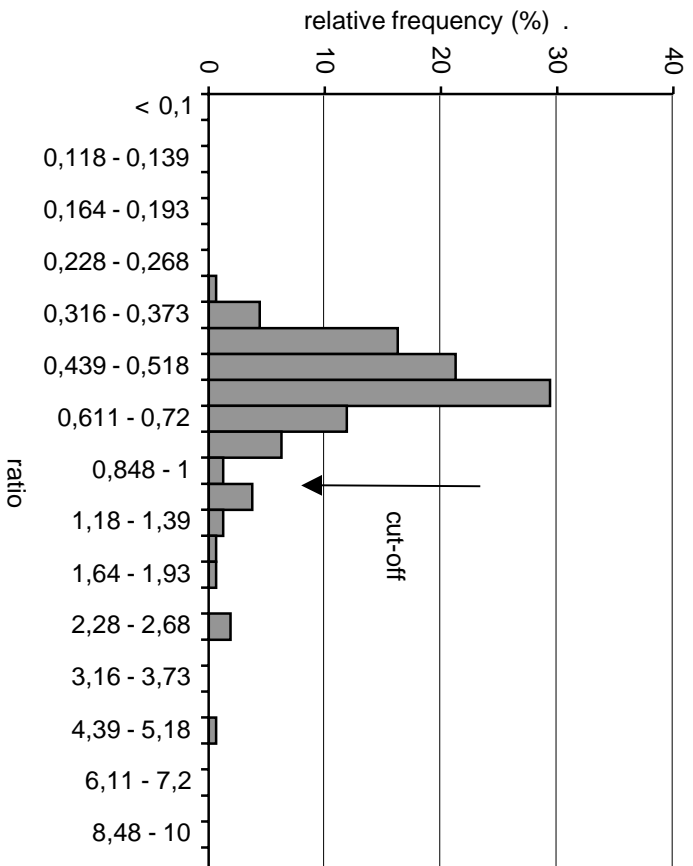

positive sera

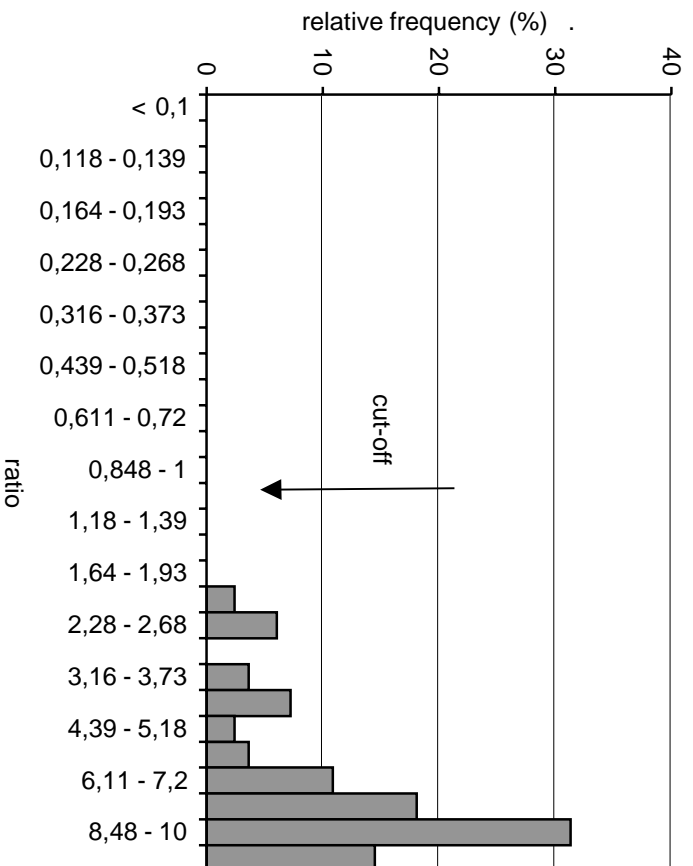

12. Warranty

IBL International guarantees that the product delivered has been thoroughly tested to ensure that its properties specified herein are fulfilled. No further warranties are given.

The performance data presented here were obtained using the procedure indicated. Any modification in the procedure may affect the results in which case IBL disclaims all warranties whether expressed, implied or statutory. Moreover, IBL accepts no liability for any damage, whether direct, indirect or consequential, which results from inappropriate use or storage of the product.








14. References

1. Nakamura, R. M., Tan, E. M.: Update on autoantibodies to intracellular antigens in systemic rheumatic diseases. *Clin Lab Med* 12 (1992), 1 - 23
2. Guma, M., Keil, L. B.: Autoantibodies to cellular antigens in systemic autoimmune diseases. *J Clin Immunoassay* 17 (1994), 98 - 107
3. Fritzler, M. J.: Clinical relevance of autoantibodies in systemic rheumatic diseases. *Mol Biol Rep* 23 (1996), 133 - 145
4. Hietarinta, M., Lassila, O.: Clinical significance of antinuclear antibodies in systemic rheumatic disease. *Ann Med* 28 (1996), 283 - 291
5. Messinger, M.: Autoantikörper bei systemischen entzündlich-rheumatischen Erkrankungen (Kollagenosen). In: L. Thomas (ed.): *Labor und Diagnose* (2005), TH-Books-Verlags-Gesellschaft, Frankfurt/Main, 1139 - 1161
6. Sommer, R., and Eitelberger, F.: Wertigkeit der Gliadin-Antikörper im Serum zur Diagnose der Zöliakie. *Wien Klin Wochenschr* 104/4 (1992), 86 - 92

15. Summary flow chart

- a. Dilute the samples 1/100 in sample buffer (100 mL, ready-to-use, orange) and mix.
- b. Dilute the wash buffer 10x-concentrate (100 mL, blue) with water and mix.
- c. Wash the wells once with 350 µL wash buffer each. Dispense 100 µL of the controls (3,0 mL each, ready-to-use, green and red) and of the diluted samples into the wells of the solid phase. Duplicate measurements are recommended. Incubate for 30 minutes at room temperature ($23 \pm 3^{\circ}\text{C}$).
- d. Wash the wells 4 times with 350 µL wash buffer each.
- e. Dispense 100 µL of the conjugate (14 mL, ready-to-use, red) into the wells. Incubate as in step c.
- f. Repeat washing step d.
- g. Dispense 100 µL of the substrate solution (14 mL, ready-to-use, black vial) per well. Incubate as in step c. Then, add 100 µL stop solution (14 mL, ready-to-use, colourless) per well and agitate the plate briefly.
- h. Immediately measure the absorbance at 450 nm.
- i. Evaluation: determine the borderline absorbance by multiplying the absorbance of the positive control with the factor quoted in the certificate of analysis. Then, calculate the ratio of the samples by dividing their absorbance by the borderline absorbance.

Symbols / Symbole / Symbôles / Símbolos / Símbolos / Σύμβολα

	Cat.-No.: / Kat.-Nr.: / No.- Cat.: / Cat.-No.: / N.º Cat.: / N.–Cat.: / Αριθμός-Κατ.:
	Lot-No.: / Chargen-Bez.: / No. Lot: / Lot-No.: / Lote N.º: / Lotto n.: / Αριθμός -Παραγωγή:
	Use by: / Verwendbar bis: / Utiliser à: / Usado por: / Usar até: / Da utilizzare entro: / Χρησιμοποιείται από:
	No. of Tests: / Kitgröße: / Nb. de Tests: / No. de Determ.: / N.º de Testes: / Quantità dei tests: / Αριθμός εξετάσεων:
	Concentrate / Konzentrat / Concentré / Concentrar / Concentrado / Concentrato / Συμπύκνωμα
	Lyophilized / Lyophilisat / Lyophilisé / Liofilizado / Liofilizado / Liofilizzato / Λυοφιλασμένο
	In Vitro Diagnostic Medical Device. / In-vitro-Diagnostikum. / Appareil Médical pour Diagnostics In Vitro. / Dispositivo Médico para Diagnóstico In Vitro. / Equipamento Médico de Diagnóstico In Vitro. / Dispositivo Medico Diagnostico In vitro. / Ιατρική συσκευή για In-Vitro Διάγνωση.
	Evaluation kit. / Nur für Leistungsbewertungszwecke. / Kit pour évaluation. / Juego de Reactivos para Evaluació. / Kit de avaliação. / Kit di evaluazione. / Κιτ Αξιολόγησης.
	Read instructions before use. / Arbeitsanleitung lesen. / Lire la fiche technique avant emploi. / Lea las instrucciones antes de usar. / Ler as instruções antes de usar. / Leggere le istruzioni prima dell'uso. / Διαβάστε τις οδηγίες πριν την χρήση.
	Keep away from heat or direct sun light. / Vor Hitze und direkter Sonneneinstrahlung schützen. / Garder à l'abri de la chaleur et de toute exposition lumineuse. / Manténgase alejado del calor o la luz solar directa. / Manter longe do calor ou luz solar directa. / Non esporre ai raggi solari. / Να φυλάσσεται μακριά από θερμότητα και άμεση επαφή με το φως του ηλίου.
	Store at: / Lagern bei: / Stocker à: / Almacene a: / Armazenar a: / Conservare a: / Αποθήκευση στους:
	Manufacturer: / Hersteller: / Fabricant: / Productor: / Fabricante: / Fabbicante: / Παραγωγός:
	Caution! / Vorsicht! / Attention! / ¡Precaución! / Cuidado! / Attenzione! / Προσοχή!
<p>Symbols of the kit components see MATERIALS SUPPLIED. Die Symbole der Komponenten sind im Kapitel KOMPONENTEN DES KITS beschrieben. Voir MATERIEL FOURNI pour les symbôles des composants du kit. Símbolos de los componentes del juego de reactivos, vea MATERIALES SUMINISTRADOS. Para símbolos dos componentes do kit ver MATERIAIS FORNECIDOS. Per i simboli dei componenti del kit si veda COMPONENTI DEL KIT. Για τα σύμβολα των συστατικών του κιτ συμβουλευτείτε το ΠΑΡΕΧΟΜΕΝΑ ΥΛΙΚΑ.</p>	

COMPLAINTS: Complaints may be submitted initially written or vocal. Subsequently they need to be filed including the test performance and results in writing in case of analytical reasons.

WARRANTY: The product is warranted to be free from material defects within the specific shelf life and to comply with product specifications delivered with the product. The product must be used according to the Intended use, all instructions given in the instructions for use and within the product specific shelf life. Any modification of the test procedure or exchange or mixing of components of different lots could negatively affect the results. These cases invalidate any claim for replacement.

LIMITATION OF LIABILITY: IN ALL CIRCUMSTANCES THE EXTENT OF MANUFACTURER'S LIABILITY IS LIMITED TO THE PURCHASE PRICE OF THE KIT(S) IN QUESTION. IN NO EVENT SHALL MANUFACTURER BE LIABLE FOR ANY INCIDENTAL OR CONSEQUENTIAL DAMAGES, INCLUDING DAMAGES FOR LOST PROFITS, LOST SALES, INJURY TO PERSON OR PROPERTY OR ANY OTHER INCIDENTAL OR CONSEQUENTIAL LOSS.

IBL International GmbH
Flughafenstrasse 52a
D-22335 Hamburg, Germany

Phone: +49 (0)40-53 28 91-0
Fax: +49 (0)40-53 28 91-11

IBL@tecan.com
www.tecan.com/ibl

Always there for you

